



CE EMC

TEST REPORT

For

Medical Station

Model: ONYX-173D; ONYX-153D

Trade Name: AAEON

Issued to

AAEON Technology Inc.

**5F, No. 135, Lane 235, Pao Chiao Rd., Hsin-Tien City,
Taipei, Taiwan, R.O.C.**

Issued by



**Compliance Certification Services Inc.
Hsintien Lab.**

**No. 165, Chungsen Road, Hsintien City
Taipei Hsien, Taiwan**

TEL: (02) 2217-0894

FAX: (02) 2217-1029

Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. Ltd. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document.



TABLE OF CONTENTS

1 TEST RESULT CERTIFICATION3

2 EUT DESCRIPTION4

3 TEST METHODOLOGY5

3.1 EUT SYSTEM OPERATION.....5

4 SETUP OF EQUIPMENT UNDER TEST6

5 FACILITIES AND ACCREDITATIONS.....7

5.1 FACILITIES7

5.2 LABORATORY ACCREDITATIONS AND LISTINGS7

6 INSTRUMENT AND CALIBRATION8

6.1 MEASURING INSTRUMENT CALIBRATION8

6.2 TEST AND MEASUREMENT EQUIPMENT8

7 LINE CONDUCTED & RADIATED EMISSION TEST.....11

7.1 LIMIT11

7.2 TEST PROCEDURE OF LINE CONDUCTED EMISSION.....12

7.3 TEST PROCEDURE OF RADIATED EMISSION14

7.4 TEST RESULTS16

8 POWER HARMONICS TEST.....18

9 POWER VOLTAGE FLUCTUATION / FLICKER TEST20

10 ELECTROSTATIC DISCHARGE (ESD) IMMUNITY TEST.....22

11 RADIATED ELECTROMAGNETIC FIELD IMMUNITY TEST.....26

12 FAST TRANSIENTS/BURST IMMUNITY TEST.....29

13 SURGE IMMUNITY TEST31

**14 CONDUCTED DISTRBANCE/INDUCED RADIO-FREQUENCY FIELD
IMMUNITY TEST.....33**

15 POWER FREQUENCY MAGNETIC FIELD IMMUNITY TEST.....35

16 VOLTAGE DIPS / SHORT INTERRUPTIONS.....37

APPENDIX I - PHOTOGRAPHS OF TEST SETUP40

APPENDIX II – TEST RESULT OF EN 61000-3-2/-347



1 TEST RESULT CERTIFICATION

Applicant: AAEON Technology Inc.
5F, No.135, Lane 235, Pao Chiao Rd., Hsin-Tien City,
Taipei, Taiwan, R.O.C.

Manufacturer: AAEON Technology Inc.
5F, No.135, Lane 235, Pao Chiao Rd., Hsin-Tien City,
Taipei, Taiwan, R.O.C.

Equipment Under Test: Medical Station

Trade Name: AAEON

Model: ONYX-173D; ONYX-153D

Detailed EUT Description: See Item 2 of this report

Date of Test: October 26, 2005 ~ November 10, 2005

| Applicable Standard | Class/Limit/Criterion | Test Result |
|---|----------------------------|-------------------------|
| EN 60601-1-2: 2001, including | | |
| EN 55011: 1998 + A1: 1999 + A2: 2002 | Group I, Class B | No non-compliance noted |
| IEC 61000-4-2: 1995 +A1: 1998 +A2: 2000 | See Item 9 of this report | No non-compliance noted |
| IEC 61000-4-3: 2002 +A1: 2002 | See Item 10 of this report | No non-compliance noted |
| IEC 61000-4-4: 1995 +A1: 2000 +A2: 2001 | See Item 11 of this report | No non-compliance noted |
| IEC 61000-4-5: 1995 + A1: 2000 | See Item 12 of this report | No non-compliance noted |
| IEC 61000-4-6: 1996 + A1: 2000 | See Item 13 of this report | No non-compliance noted |
| IEC 61000-4-8: 1993 + A1: 2000 | See Item 14 of this report | No non-compliance noted |
| IEC 61000-4-11: 1994 + A1: 2000 | See Item 15 of this report | No non-compliance noted |
| EN 61000-3-2: 2000 | Class D | No non-compliance noted |
| EN 61000-3-3: 1995 + A1: 2001 | Limit | No non-compliance noted |
| Deviation from Applicable Standard | | |
| None | | |

The above equipment was tested by Compliance Certification Services Inc. for compliance with the requirements set forth in the EMC Directive 93/42/EEC and the technical standards mentioned above. The results of testing in this report apply only to the product/system, which was tested. Other similar equipment will not necessarily produce the same results due to production tolerance and measurement uncertainties.

Approved by:

David Wang
Manager of Hsintien Laboratory
Compliance Certification Services Inc.

Reviewed by:

Vince Chiang
Assistant Manager of Hsintien Laboratory
Compliance Certification Services Inc.

**2 EUT DESCRIPTION**

| | |
|--------------------------------|--|
| Product | Medical Station |
| Trade Name | AAEON |
| Model | ONYX-173D; ONYX-153D |
| Housing Type | Plastic w/ metal plate |
| EUT Power Rating | 15VDC from AC Adaptor |
| AC Power During Test | 230VAC / 50Hz to AC Adaptor |
| AC Adaptor Manufacturer | FSP |
| AC Adaptor Model Number | FSP105-AGB |
| AC Adaptor Power Rating | I/P: 100-240VAC 50-60Hz O/P: 15VDC |
| AC Power Cord Type | Unshielded, 1.8m (Non-detachable) |
| DC Power Cord Type | Unshielded, 1.9m (Detachable, with a core) |
| OSC/Clock Frequencies | 14.31818MHz; 25MHz; 32.768kHz |

EUT DIFFERENCE

| | Model Name | Differences (Faceplate) | Differences (Panel M/N) | Tested (Checked) |
|-------------------|------------|-------------------------|-------------------------|-------------------------------------|
| Original | ONYX-173D | 17" TFT LCD | CLAA17EA-07Y | <input checked="" type="checkbox"/> |
| Additional | ONYX-153D | 15" TFT LCD | CLAA150XP03 | <input checked="" type="checkbox"/> |

I/O PORT OF EUT

| I/O PORT TYPE | Q' TY | TESTED WITH |
|--------------------------|-------|-------------|
| 1). PIO Port | 1 | 1 |
| 2). SIO Port | 3 | 3 |
| 3). PS/2 Keyboard Port | 1 | 1 |
| 4). PS/2 Mouse Port | 1 | 1 |
| 5). VIDEO-OUT Port (VGA) | 1 | 1 |
| 6). AUDIO IN Port | 2 | 2 |
| 7). Earphone Port | 1 | 1 |
| 8). Microphone Port | 1 | 1 |
| 9). LAN Port | 1 | 1 |
| 10). USB Port | 5 | 5 |
| 11). S-VIDEO OUT Port | 1 | 1 |
| 12). CF Slot | 1 | 1 |
| 13). SD Slot | 1 | 1 |
| 14). SM Slot | 1 | 1 |
| 15). Memory Stick Slot | 1 | 1 |

Note: None.



3 TEST METHODOLOGY

3.1 EUT SYSTEM OPERATION

1. Windows 2000 boots system.
2. Run Emctest.exe to activate all peripherals and display “H” pattern on monitor screen.
3. Run Winemc.exe and choose “E:/ & F:/ & G:/ & H:/ & I:/ & J:/ & K:/ & L:/ & I:” to test EUT.
4. Run Winemc.exe and choose media player to play music.
5. Press the start menu, select executive and type ping 192.168.0.2 –t (EUT), ping 192.168.0.1 –t (Server PC).

Note: Test program is self-repeating throughout the test.

3.2 DECISION OF FINAL TEST MODE

1. The following test mode(s) were scanned during the preliminary test:

Mode(s):

| | |
|----|--|
| 1. | ONYX-173D / PANEL + LCD / 1280X1024, VF=75Hz |
| 2. | ONYX-173D / PANEL + LCD / 1024X768, VF=70Hz |
| 3. | ONYX-173D / PANEL + LCD / 800X600, VF=60Hz |
| 4. | ONYX-173D / PANEL + TV / 1024X768, VF=60Hz |
| 5. | ONYX-173D / PANEL + TV / 800X600, VF=60Hz |
| 6. | ONYX-153D / PANEL + LCD / 1280X1024, VF=75Hz |

2. After the preliminary scan, the following test mode was found to produce the highest emission level.

Conduction: Mode 1

Radiation: Mode 1

Then, the EUT configuration and cable configuration of the above highest emission mode was chosen for all final test items.



4 SETUP OF EQUIPMENT UNDER TEST

Setup Diagram

See test photographs attached in Appendix I for the actual connections between EUT and support equipment.

Support Equipment

EUT Devices:

| No | Equipment | Model # | Trade Name |
|----|----------------|-----------|----------------------|
| 1 | CPU (1.6GHz) | N/A | Genuine Intel Mobile |
| 2 | DVD ROM | DV-28SL | TEAC |
| 3 | Hard Disk | MHT2020AT | FUJITSU |
| 4 | Memory (512MB) | DDR333MHz | DSL |

Peripherals Devices:

| No | Equipment | Model | Serial No. | FCC ID/ BSMI ID | Trade Name | Data Cable | Power Cord |
|----|---------------|-------------|-----------------|-----------------------|--------------|-------------------------------|------------------------------|
| 1 | Ear / Mic | MSB301 | N/A | N/A | e-Sense | Unshielded, 1.8m | N/A |
| 2 | Player | RQ-L317 | N/A | N/A | PANASONIC | Unshielded, 1.8m | N/A |
| 3 | USB 2.0 HDD | F12-U | N/A | BSMI ID: 4912A002 | TeraSys | Shielded, 2.0m | Unshielded, 1.8m with a core |
| 4 | USB 2.0 HDD | F12-U | N/A | BSMI ID: 4912A002 | TeraSys | Shielded, 2.0m | Unshielded, 1.8m with a core |
| 5 | USB 2.0 HDD | F12-U | N/A | BSMI ID: 4912A002 | TeraSys | Shielded, 2.0m | Unshielded, 1.8m with a core |
| 6 | USB 2.0 HDD | F12-U | N/A | BSMI ID: 4912A002 | TeraSys | Shielded, 2.0m | Unshielded, 1.8m with a core |
| 7 | USB 2.0 HDD | F12-U | N/A | BSMI ID: 4912A002 | TeraSys | Shielded, 2.0m | Unshielded, 1.8m with a core |
| 8 | PS/2 Mouse | M071KC | 443029438 | BSMI: R41108 DoC | DELL | Shielded, 1.8m | N/A |
| 9 | PS/2 Keyboard | SK-8110 | N/A | BSMI: T3A002 DoC | DELL | Shielded, 1.8m | N/A |
| 10 | Printer | C60 | N/A | BSMI ID: 3902E006 | EPSON | Shielded, 1.8 m | Unshielded, 1.8m |
| 11 | Monitor (TV) | KD17NS | 7728 | BSMI: R33475 | SAMAUNG | Shielded, 1.8m | Unshielded, 1.8m |
| 12 | Monitor | 171T | GH17H4LT702622L | R33475 | SAMSUNG | Shielded, 1.8m with two cores | Unshielded, 1.8m |
| 13 | Modem | 5JEG4033MKO | N/A | 5RJTAI-35500-M5-E | TOP-SOLUTION | Shielded, 1.8m | Unshielded, 1.8m |
| 14 | Modem | 5JEG4033MKO | N/A | 5RJTAI-35500-M5-E | TOP-SOLUTION | Shielded, 1.8m | Unshielded, 1.8m |
| 15 | Modem | 5JEG4033MKO | N/A | 5RJTAI-35500-M5-E | TOP-SOLUTION | Shielded, 1.8m | Unshielded, 1.8m |
| 16 | Server PC | 5420GC | 1D23KMDWM08 | DoC BSMI ID: 3892B894 | COMPAQ | Unshielded, 10m | Unshielded, 1.8m |
| 17 | SD Card | N/A | N/A | N/A | N/A | N/A | N/A |
| 18 | SM Card | N/A | N/A | N/A | N/A | N/A | N/A |
| 19 | MS Card | N/A | N/A | N/A | N/A | N/A | N/A |
| 20 | CF Card | N/A | N/A | N/A | N/A | N/A | N/A |

Note: All the above equipment/cables were placed in worse case positions to maximize emission signals during emission test.

Grounding: Grounding was in accordance with the manufacturer's requirements and conditions for the intended use.

5 FACILITIES AND ACCREDITATIONS

5.1 FACILITIES








All measurement facilities (except above 1GHz measurement frequency of IEC 61000-4-3) used to collect the measurement data are located at CCS Taiwan Hsintien Lab at No. 165, Chunghsen Road, Hsintien City, Taipei Hsien, Taiwan.

The measurement facilities of IEC 61000-4-3 frequency rang above 1GHz are located at CCS Taiwan Wuku Lab. at No. 11, Wu-Kung 6 Rd., Wu-Ku Hsiang, Wu-Ku Industrial District, Taipei Hsien, Taiwan

The measurement facilities are constructed in conformance with the requirements of CISPR 16-1, ANSI C63.4 and other equivalent standards.

5.2 LABORATORY ACCREDITATIONS AND LISTINGS

The test facilities used to perform Electromagnetic compatibility tests are registered or accredited by the organizations listed in the following table which includes the recognized scope specifically.

| Country | Agency | Scope of Accreditation | Logo |
|---------|-----------------|--|---|
| USA | A2LA | CFR 47, FCC Part 15/18 using ANSI 63.4; AS/NZS 3548; VCCI V3; CNS 13438; CNS 13439; CNS 13783; CNS 14115; CISPR 11/EN 55011; CISPR 14-1/EN 55014-1; CISPR 15/EN 55015; CISPR 22/EN 55022; EN 50081-1/EN 61000-6-3; EN 50082-1/EN 61000-6-4; IEC/EN 61000-4-2, IEC/EN 61000-4-3, IEC/EN 61000-4-4, IEC/EN 61000-4-5, IEC/EN 61000-4-6, IEC/EN 61000-4-8, IEC/EN 61000-4-11, IEC/EN 61000-3-2, IEC/EN 61000-3-3; CISPR 24/EN 55024; CISPR 14-2/EN 55014-2; EN 50081-2/EN 61000-6-1; EN 50082-2/EN 61000-6-2. |  824.01 |
| USA | FCC | 3/10 meter Open Area Test Sites to perform FCC Part 15/18 measurements |  250366 |
| Japan | VCCI | 3/10 meter Open Area Test Sites and Line Conducted Test Room to perform conducted/radiated measurements |  R-1434/1630~4 C-1511/1882 |
| Norway | NEMKO | EN 50081-1/2, EN 50082-1/2, IEC 61000-6-1/2/3/4, EN 50091-2, EN 50130-4, EN 55011, EN 55013, EN 55014-1/2, EN 55015, EN 55022, EN 55024, EN 61000-3-2/3, EN 61326-1, IEC 61000-4-2/3/4/5/6/8/11, Cisprr 16-1/2/3/4 |  ELA 103 |
| Taiwan | CNLA | 47 CFR FCC Part 15 Subpart B, EN 61000-3-2, EN 61000-3-3, CNS 13439, CNS 13783-1, CNS 13438, AS/NZS 3548, VCCI, CNS 13022-1/2/3, EN 55022, EN 55013, EN 55014-1, EN 61000-4-2/3/4/5/6/8/11, ENV 50204, ENV 50141, ENV 50142 |  1108 ILAC MRA |
| Taiwan | BSMI | CNS 13438, CNS 13783-1, CNS 13439 |  SL2-IN-E-0005 SL2-A1-E-0005 SL2-R1-E-0005 SL2-R2-E-0005 |
| Canada | Industry Canada | RSS212, Issue 1 |  IC 5742 |

Note: No part of this report may be used to claim or imply product endorsement by CNLA, A2LA or other government agency.



6 INSTRUMENT AND CALIBRATION

6.1 MEASURING INSTRUMENT CALIBRATION

The measuring equipment utilized to perform the tests documented in this report has been calibrated once a year or in accordance with the manufacturer's recommendations, and is traceable to recognized national standards.

6.2 TEST AND MEASUREMENT EQUIPMENT

The following list contains measurement equipment used for testing. The equipment conforms to the requirement of CISPR 16-1, ANSI C63.2 and other required standards.

Calibration of all test and measurement, including any accessories that may effect such calibration, is checked frequently to ensure the accuracy. Adjustments are made and correction factors are applied in accordance with the instructions contained in the respective manual.

Equipment Used for Emission Measurement

| Open Area Test Site # I | | | | |
|-------------------------|-----------|-----------|---------------|-------------------------|
| EQUIPMENT | MFR | MODEL | SERIAL NUMBER | CAL. DUE |
| SITE NSA | CCS | I Site | N/A | 10/14/2006 |
| MEASURE RECEIVER | SCHAFFNER | SCR3501 | 338 | 06/27/2006 |
| SPECTRUM ANALYZER | ADVANTEST | R3132 | 120900008 | No Calibration Required |
| ANTENNA | SCHAFFNER | CBL 6112B | 2809 | 09/23/2006 |
| AMPLIFIER | SCHAFFNER | CPA9231A | 3626 | 10/08/2006 |
| CABLE | BELDEN | 9913 | N-TYPE #I2 | 02/18/2006 |
| ATTENUATOR | MCL | UNAT-6 | AT06-3 | 10/08/2006 |
| THERMO-HYGRO METER | TFA | N/A | NO.2 | 11/02/2006 |

Note: The measurement uncertainty is less than +/- 3.36dB, which is evaluated as per the NAMAS NIS 81 and CISPR/A/291/CDV.

| Conducted Emission Test Site # B | | | | |
|----------------------------------|----------|---------|---------------|------------|
| EQUIPMENT | MFR | MODEL | SERIAL NUMBER | CAL. DUE |
| TEST RECEIVER | R&S | ESHS10 | 843743/015 | 03/31/2006 |
| LISN (EUT) | EMCO | 3825/2 | 9106-1810 | 01/16/2006 |
| LISN | EMCO | 3825/2 | 1382 | 01/16/2006 |
| BNC CABLE | MIYAZAKI | 5D-FB | BNC B1 | 07/14/2006 |
| Pulse Limiter | R&S | ESH3-Z2 | 100374 | 08/25/2006 |
| THERMO-HYGRO METER | TOP | HA-202 | 9303-3 | 03/02/2006 |

Note: The measurement uncertainty is less than +/- 2.83dB, which is evaluated as per the NAMAS NIS 81 and CISPR/A/291/CDV.



| Power Harmonic & Voltage Fluctuation/Flicker Test Site (EN 61000-3-2&-3-3) | | | |
|---|------------------|-------------------|-------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / Signal Conditioning Unit | CCN 1000-1 | 72122 | 12/05/2005 |
| Schaffner / 5KVA AC Power Source | NSG 1007 | 55131 | No Calibration Required |

Equipment Used for Immunity Measurement

| ESD Test Site (EN 61000-4-2) | | | |
|-------------------------------------|------------------|-------------------|-----------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / ESD Simulator | NSG 438 | 129 | 04/20/2006 |
| Sato / Aneroid Barometer | 7610-20 | 89090 | 08/29/2006 |
| TOP / Thermo-Hygro meter | HA-202 | 9303-1 | 03/02/2006 |

| Radiated Electromagnetic Field Immunity Test Site (EN 61000-4-3) | | | |
|---|------------------|-------------------|-------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Calibration of Field | Chamber#RS | RS3H-7 / RS3V-7 | 07/01/2006 |
| Agilent / Signal Generator | E4421B | MY43350597 | 05/16/2006 |
| AR / Electric Field Probe | FP6001 | 305650 | 02/03/2006 |
| Boonton / RF Voltmeter | 9200B | 328001AE | 02/23/2006 |
| BNC / Function Generator | 625A | 25451 | 02/17/2006 |
| AR / Amplifier | 100W1000M1 | 17564 | No Calibration Required |
| Werlatone Inc. / Direction Coupler | C2630 | 4121 | No Calibration Required |
| Frankonia / Broadband Antenna | BTA-M | 030001M | No Calibration Required |
| TOP / Thermo-Hygro meter | HA-202 | 9303-2 | 03/02/2006 |

| Fast Transients/Burst Test Site (EN 61000-4-4) | | | |
|---|------------------|-------------------|-------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / EFT Generator | BEST EMC V2.3 | 200031A024SC | 11/09/2005 |
| Schaffner / Capacitive Clamp | N/A | N/A | No Calibration Required |



| Surge Immunity Test Site (EN 61000-4-5) | | | |
|---|------------------|-------------------|----------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / Surger Generator | BEST EMC V2.3 | 200031A024SC | 11/09/2005 |
| Schaffner / Signal and Data Lines Coupling Network | CDN118 | 19328 | No Calibration Required |

| CS test (EN 61000-4-6) | | | |
|-------------------------------|------------------|-------------------|----------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / RF Generator | NSG 2070-1 | 1061 | 08/03/2006 |
| Schaffner / CDN | CDN M316 | 19600 | 08/02/2006 |
| Schaffner / CDN | CDN M216 | 19294 | 08/02/2006 |
| FCC / CDN | FCC-801-M3-16A | 99122 | 08/02/2006 |
| Schaffner / EM Clamp | KEMZ 801 | 19227 | 02/23/2006 |
| Schaffner / CDN | CDN T002 | 15881 | 01/13/2006 |
| FCC / CDN | FCC-801-T8-RJ45 | 04025 | 06/23/2006 |
| Schaffner / Attenuator | INA2070-1 | 2061 | No Calibration Required |
| FCC / CDN | FCC-801-T4-RJ45 | 04031 | 08/02/2006 |

| Power Frequency Magnetic Field Immunity test (EN 61000-4-8) | | | |
|--|------------------|-------------------|----------------------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / Induction Coil Interface | INA 21141 | 6009 | No Calibration Required |
| Schaffner / 5KVA AC Power Source | NSG 1007 | 55131 | No Calibration Required |
| Sypris / Magnetic Field Meter | 4080 | 0247 | 01/19/2006 |

| Voltage Dips/Short Interruption and Voltage Variation Immunity test (EN 61000-4-11) | | | |
|--|------------------|-------------------|-----------------|
| Manufacturer/Type | Model No. | Serial No. | Cal. Due |
| Schaffner / Dips/Interruption/Variations Tester | BEST EMC V2.3 | 200031A024SC | 11/09/2005 |
| Protronix / Digital Power Meter | 1201 | 201091 | 08/24/2006 |



7 LINE CONDUCTED & RADIATED EMISSION TEST

7.1 LIMIT

Maximum permissible level of Line Conducted Emission

| Frequency (MHZ) | Class A (dB μ V) | | Class B (dB μ V) | |
|--------------------|----------------------|---------|----------------------|---------|
| | Quasi-peak | Average | Quasi-peak | Average |
| 0.15 - 0.5 | 79 | 66 | 66 - 56 | 56 - 46 |
| 0.50 - 5.0 | 73 | 60 | 56 | 46 |
| 5.0 - 30.0 | 73 | 60 | 60 | 50 |

Note: The lower limit shall apply at the transition frequency.

Maximum permissible level of Radiated Emission measured at 10 meter

| Frequency (MHZ) | Class A (dB μ V/m) | Class B (dB μ V/m) |
|--------------------|------------------------|------------------------|
| | Quasi-peak | Quasi-peak |
| 30 - 230 | 40 | 30 |
| 230 - 1000 | 47 | 37 |

Note: The lower limit shall apply at the transition frequency.



7.2 TEST PROCEDURE OF LINE CONDUCTED EMISSION

Procedure of Preliminary Test

- The EUT was set up as per the test configuration to simulate typical usage per the user's manual. When the EUT is a tabletop system, a wooden table with a height of 0.8 meters is used and is placed on the ground plane as per EN 55011 (see Test Facility for the dimensions of the ground plane used). When the EUT is floor-standing equipment, it is placed on the ground plane that has a 3-12 mm non-conductive covering to insulate the EUT from the ground plane.
- Support equipment, if needed, was placed as per EN 55011.
- All I/O cables were positioned to simulate typical actual usage as per EN 55011.
- The test equipment EUT installed received AC power, 230VAC/50Hz, through a Line Impedance Stabilization Network (LISN), which supplied power source and was grounded to the ground plane.
- All support equipment received power from a second LISN.
- The EUT test program was started. Emissions were measured on each current carrying line of the EUT using an EMI Test Receiver connected to the LISN powering the EUT.
- The Receiver scanned from 150kHz to 30MHz for emissions in each of the test modes.
- During the above scans, the emissions were maximized by cable manipulation.
- The test mode(s) described in Item 3.2 were scanned during the preliminary test.
- After the preliminary scan, we found the test mode described in Item 3.2 producing the highest emission level.
- The EUT configuration and cable configuration of the above highest emission levels were recorded for reference of the final test.

Procedure of Final Test

- EUT and support equipment were set up on the test bench as per the configuration with highest emission level in the preliminary test.
- A scan was taken on both power lines, Line 1 and Line 2, recording at least the six highest emissions. Emission frequency and amplitude were recorded into a computer in which correction factors were used to calculate the emission level and compare reading to the applicable limit. If EUT emission level was less -2dB to the Average limit in Q.P. mode, then the emission signal was re-checked using an Average detector.
- The test data of the worst-case condition(s) was recorded.



Data Sample:

| Freq. MHz | Read Level dBuV | Factor dB | Level dBuV | Limit dBuV | Over Limit dB | Reading Type (P/Q/A) | Line (L1/L2) |
|-----------|-----------------|-----------|------------|------------|---------------|----------------------|--------------|
| x.xx | 42.95 | 0.55 | 43.50 | 56 | -12.50 | Q | L1 |

- Freq. = Emission frequency in MHz
- Read Level = Uncorrected Analyzer/Receiver reading
- Factor = Insertion loss of LISN + Cable Loss
- Level = Read Level + Factor
- Limit = Limit stated in standard
- Over Limit = Reading in reference to limit
- P = Peak Reading
- Q = Quasi-peak Reading
- A = Average Reading
- L1 = Hot side
- L2 = Neutral side

Calculation Formula

Over Limit (dB) = Level (dBuV) – Limit (dBuV)



7.3 TEST PROCEDURE OF RADIATED EMISSION

Procedure of Preliminary Test

- The equipment was set up as per the test configuration to simulate typical usage per the user's manual. When the EUT is a tabletop system, a wooden turntable with a height of 0.8 meters is used which is placed on the ground plane. When the EUT is floor-standing equipment, it is placed on the ground plane that has a 3-12 mm non-conductive covering to insulate the EUT from the ground plane.
- Support equipment, if needed, was placed as per EN 55011.
- All I/O cables were positioned to simulate typical usage as per EN 55011.
- The EUT received AC power source, 230VAC/50Hz, from the outlet socket under the turntable. All support equipment received power from another socket under the turntable.
- The antenna was placed at 10 meter away from the EUT as stated in EN 55011. The antenna connected to the Spectrum Analyzer via a cable and at times a pre-amplifier would be used.
- The Analyzer / Receiver quickly scanned from 30MHz to 1000MHz. The EUT test program was started. Emissions were scanned and measured rotating the EUT to 360 degrees and positioning the antenna 1 to 4 meters above the ground plane, in both the vertical and the horizontal polarization, to maximize the emission reading level.
- The test mode(s) described in Item 3.2 were scanned during the preliminary test:
- After the preliminary scan, we found the test mode described in Item 3.2 producing the highest emission level.
- The EUT and cable configuration, antenna position, polarization and turntable position of the above highest emission level were recorded for the final test.

Procedure of Final Test

- EUT and support equipment were set up on the turntable as per the configuration with highest emission level in the preliminary test.
- The Analyzer / Receiver scanned from 30MHz to 1000MHz. Emissions were scanned and measured rotating the EUT to 360 degrees, varying cable placement and positioning the antenna 1 to 4 meters above the ground plane, in both the vertical and the horizontal polarization, to maximize the emission reading level.
- Recorded at least the six highest emissions. Emission frequency, amplitude, antenna position, polarization and turntable position were recorded into a computer in which correction factors were used to calculate the emission level and compare reading to the applicable limit and only Q.P. reading is presented.
- The test data of the worst-case condition(s) was recorded.



Data Sample:

| Freq. MHz | Read Level dBuV | Factor dB/m | Level dBuV/m | Limit dBuV/m | Over Limit dB | Reading Type (P/Q/A) | Pol. (H/V) |
|-----------|-----------------|-------------|--------------|--------------|---------------|----------------------|------------|
| x.xx | 14.0 | 12.2 | 26.2 | 30 | -3.8 | Q | H |

- Freq. = Emission frequency in MHz
- Read Level = Uncorrected Analyzer/Receiver reading
- Factor = Antenna Factor + Cable Loss + Attenuator (3/6/10dB) – Amplifier Gain
- Level = Read Level + Factor
- Limit = Limit stated in standard
- Over Limit = Reading in reference to limit
- P = Peak Reading
- Q = Quasi-peak Reading
- A = Average Reading
- H = Antenna Polarization: Horizontal
- V = Antenna Polarization: Vertical

Calculation Formula

Over Limit (dB) = Level (dBuV/m) – Limit (dBuV/m)



7.4 TEST RESULTS

Line Conducted Emission

Model: ONYX-173D

Test Mode: Mode 1

Temperature: 23°C

Humidity: 57% RH

Test Results: Passed

Tested by: WEBBER JUNG

(The chart below shows the highest readings taken from the final data)

| Six Highest Conducted Emission Readings | | | | | | | |
|---|-------------------|-------------|--------------|-------------------|-----------------|----------------------|--------------|
| Frequency Range Investigated | | | | 150 kHz to 30 MHz | | | |
| Freq (MHz) | Read Level (dBuV) | Factor (dB) | Level (dBuV) | Limit Line (dBuV) | Over Limit (dB) | Reading Type (P/Q/A) | Line (L1/L2) |
| 0.421 | 31.23 | 9.97 | 41.20 | 57.42 | -16.22 | P | L1 |
| 0.253 | 33.97 | 9.97 | 43.94 | 61.64 | -17.70 | P | L2 |
| 0.332 | 34.17 | 9.97 | 44.14 | 59.40 | -15.26 | P | L2 |
| 0.421 | 34.49 | 9.97 | 44.46 | 57.42 | -12.96 | P | L2 |
| 0.499 | 32.60 | 9.98 | 42.58 | 56.01 | -13.43 | P | L2 |
| 12.188 | 31.44 | 10.37 | 41.81 | 60.00 | -18.19 | P | L2 |

NOTE: The emission level was or more than 2dB below the Average limit, so no re-check anymore.



Radiated Emission

Model: ONYX-173D

Test Mode: Mode 1

Temperature: 25°C

Humidity: 61% RH

Test Results: Passed

Tested by: MARK HSU

(The chart below shows the highest readings taken from the final data)

| Six Highest Radiated Emission Readings | | | | | | | |
|---|--------------------------|----------------------|-----------------------|----------------------------------|------------------------|-----------------------------|-------------------|
| Frequency Range Investigated | | | | 30 MHz to 1000 MHz at 10m | | | |
| Freq (MHz) | Read Level (dBuV) | Factor (dB/m) | Level (dBuV/m) | Limit Line (dBuV/m) | Over Limit (dB) | Reading Type (P/Q/A) | Pol. (H/V) |
| 125.008 | 35.70 | -9.25 | 26.45 | 30.00 | -3.55 | Q | V |
| 135.310 | 33.00 | -9.63 | 23.37 | 30.00 | -6.63 | Q | V |
| 160.010 | 37.50 | -11.07 | 26.43 | 30.00 | -3.57 | Q | V |
| 233.500 | 40.50 | -9.20 | 31.30 | 37.00 | -5.70 | Q | V |
| 233.500 | 38.90 | -9.20 | 29.70 | 37.00 | -7.30 | Q | H |
| 480.041 | 32.30 | -2.35 | 29.95 | 37.00 | -7.05 | Q | H |

NOTE: None.




8 POWER HARMONICS TEST

Port : AC Power Port
Basic Standard : EN 61000-3-2 (2000)
Limits : CLASS A; CLASS B; CLASS C; CLASS D
Tested by : KEVIN CHANG
Temperature : 18°C
Humidity : 53%

Limit:

| Limits for Class A equipment | | Limits for Class D equipment | | |
|------------------------------|--------------------------------------|------------------------------|--|--------------------------------------|
| Harmonics Order n | Max. permissible harmonics current A | Harmonics Order n | Max. permissible harmonics current per watt mA/W | Max. permissible harmonics current A |
| Odd harmonics | | Odd Harmonics only | | |
| 3 | 2.30 | 3 | 3.4 | 2.30 |
| 5 | 1.14 | 5 | 1.9 | 1.14 |
| 7 | 0.77 | 7 | 1.0 | 0.77 |
| 9 | 0.40 | 9 | 0.5 | 0.40 |
| 11 | 0.33 | 11 | 0.35 | 0.33 |
| 13 | 0.21 | 13 | 0.30 | 0.21 |
| 15<=n<=39 | 0.15x15/n | 15<=n<=39 | 3.85/n | 0.15x15/n |
| Even harmonics | | | | |
| 2 | 1.08 | | | |
| 4 | 0.43 | | | |
| 6 | 0.30 | | | |
| 8<=n<=40 | 0.23x8/n | | | |

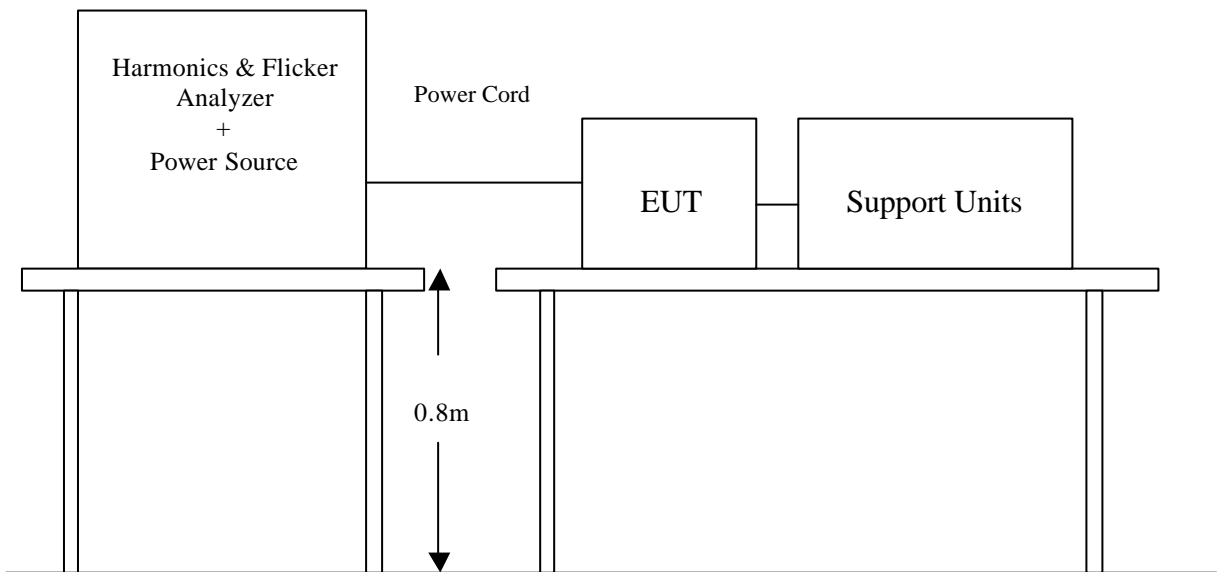

Block Diagram of Test Setup:

Test Procedure:

- a. The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the maximum harmonic components under normal operating conditions for each successive harmonic component in turn.
- b. The correspondent test program of test instrument to measure the current harmonics emanated from EUT is chosen. The measure time shall be not less than the time necessary for the EUT to be exercised.

Test Result : (See Appendix II for details)

| |
|--|
| <input checked="" type="checkbox"/> PASS <input type="checkbox"/> FAIL |
| Note: None. |


9 POWER VOLTAGE FLUCTUATION / FLICKER TEST

Port : AC Power Port
Basic Standard : EN 61000-3-3 (1995 + A1: 2001)
Limits : § of EN 61000-3-3
Tested by : KEVIN CHANG
Temperature : 18°C
Humidity : 53%

Limit:

| TEST ITEM | LIMIT | REMARK |
|---------------|-------|--|
| P_{st} | 1.0 | P_{st} means short-term flicker indicator. |
| P_{lt} | 0.65 | P_{lt} means long-term flicker indicator. |
| T_{dt} (ms) | 500 | T_{dt} means maximum time that dt exceeds 3 %. |
| d_{max} (%) | 4% | d_{max} means maximum relative voltage change. |
| dc (%) | 3.3% | dc means relative steady-state voltage change |

Block Diagram of Test Setup:

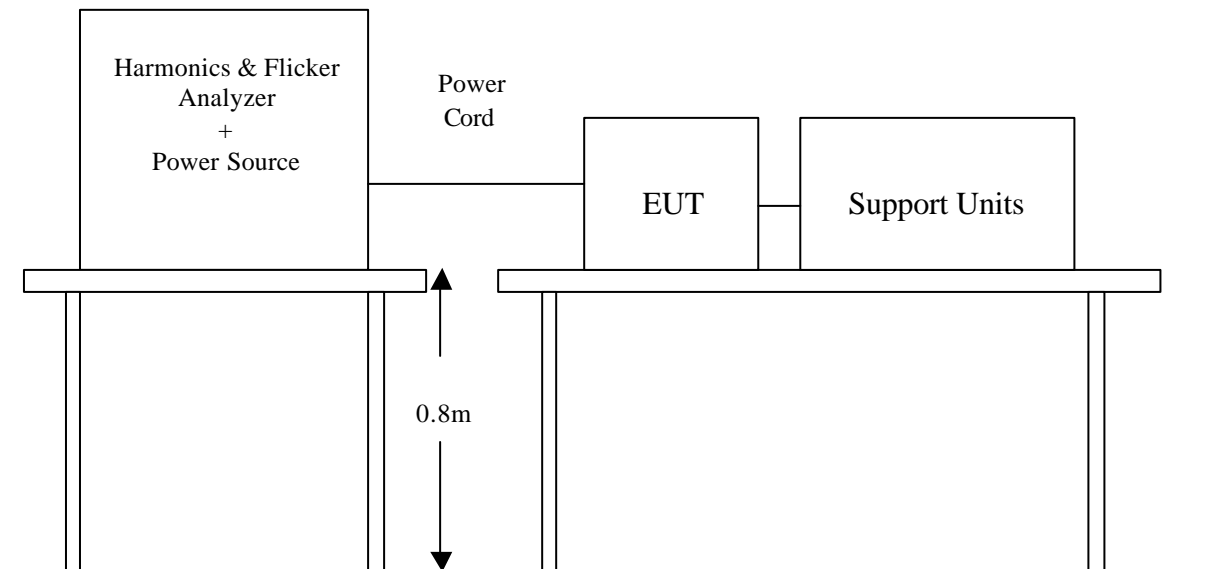



Test Procedure:

- a. The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the most unfavorable sequence of voltage changes under normal operating conditions.
- b. During the flick measurement, the measure time shall include that part of whole operation cycle in which the EUT produce the most unfavorable sequence of voltage changes. The observation period for short-term flicker indicator is 10 minutes and the observation period for long-term flicker indicator is 2 hours.

Test Result: (See Appendix II for details)

| Test Parameter | Measurement Value | Limit | Result |
|----------------|-------------------|-------|--------|
| P_{st} | 0.001 | 1.0 | Pass |
| P_{lt} | 0.001 | 0.65 | Pass |
| T_{dt} (ms) | 0 | 500 | Pass |
| d_{max} (%) | 0 | 4% | Pass |
| dc (%) | 0 | 3.3% | Pass |


Note: None.

10 ELECTROSTATIC DISCHARGE (ESD) IMMUNITY TEST

| | |
|------------------------------|---|
| Port | : Enclosure |
| Basic Standard | : IEC/EN 61000-4-2 |
| Test Level | : $\pm 2, 4, 8$ kV (Air Discharge) : $\pm 2, 4, 6$ kV (Contact Discharge) |
| Performance Criterion | : The Equipment or System shall be able to provide the essential performance and remain safe. |
| Tested by | : BENSON YANG |
| Temperature | : 18°C |
| Humidity | : 53% RH |
| Pressure | : 1010mbar |

Block Diagram of Test Setup:

(The 470 k Ω resistors are installed per standard requirement.)

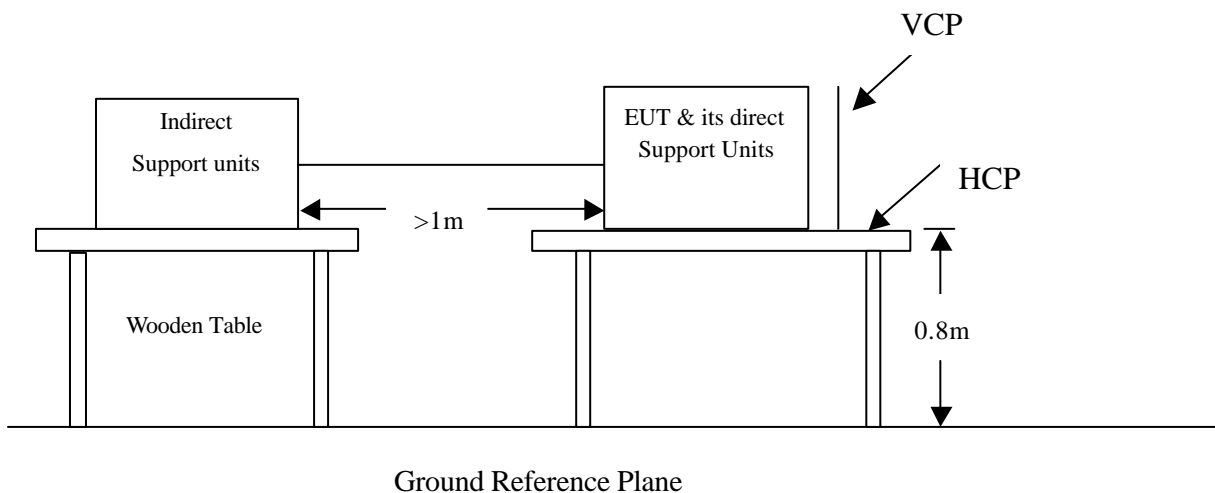

**Test Procedure:**

The electrostatic discharges were applied as follows:

| Amount of Discharges | Voltage | Coupling | Result (Pass/Fail) |
|----------------------|--------------|--------------------------------|--------------------|
| 20 / Point | ± 2, 4, 8 kV | Air Discharge | Pass |
| 20 / Point | ± 2, 4, 6 kV | Contact Discharge | Pass |
| 20 / Point | ± 2, 4, 6 kV | Indirect Discharge HCP | Pass |
| 20 / Point | ± 2, 4, 6 kV | Indirect Discharge VCP (Front) | Pass |
| 20 / Point | ± 2, 4, 6 kV | Indirect Discharge VCP (Left) | Pass |
| 20 / Point | ± 2, 4, 6 kV | Indirect Discharge VCP (Back) | Pass |
| 20 / Point | ± 2, 4, 6 kV | Indirect Discharge VCP (Right) | Pass |

****For the tested points to EUT, please refer to attached page.**

(Blue Arrow Mark For Contact Discharge And Red Arrow Mark For Air Discharge)

Observation: No function degraded during the tests.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer's presets)
- Change of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.

For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer's specifications) that does not affect ESSENTIAL PERFORMANCE or safety.



The Tested Points of EUT

Photo 1 of 4



Photo 2 of 4





Photo 3 of 4




Photo 4 of 4



11 RADIATED ELECTROMAGNETIC FIELD IMMUNITY TEST

| | |
|------------------------------|---|
| Port | : Enclosure |
| Basic Standard | : IEC/EN 61000-4-3 |
| Requirements | : 3 V/m with 80% AM, 1kHz Modulation. |
| Performance Criterion | : The Equipment or System shall be able to provide the essential performance and remain safe. |
| Tested by | : BENSON YANG |
| Temperature | : 18°C |
| Humidity | : 53% RH |
| Pressure | : 1010mbar |

Block Diagram of Test Setup:

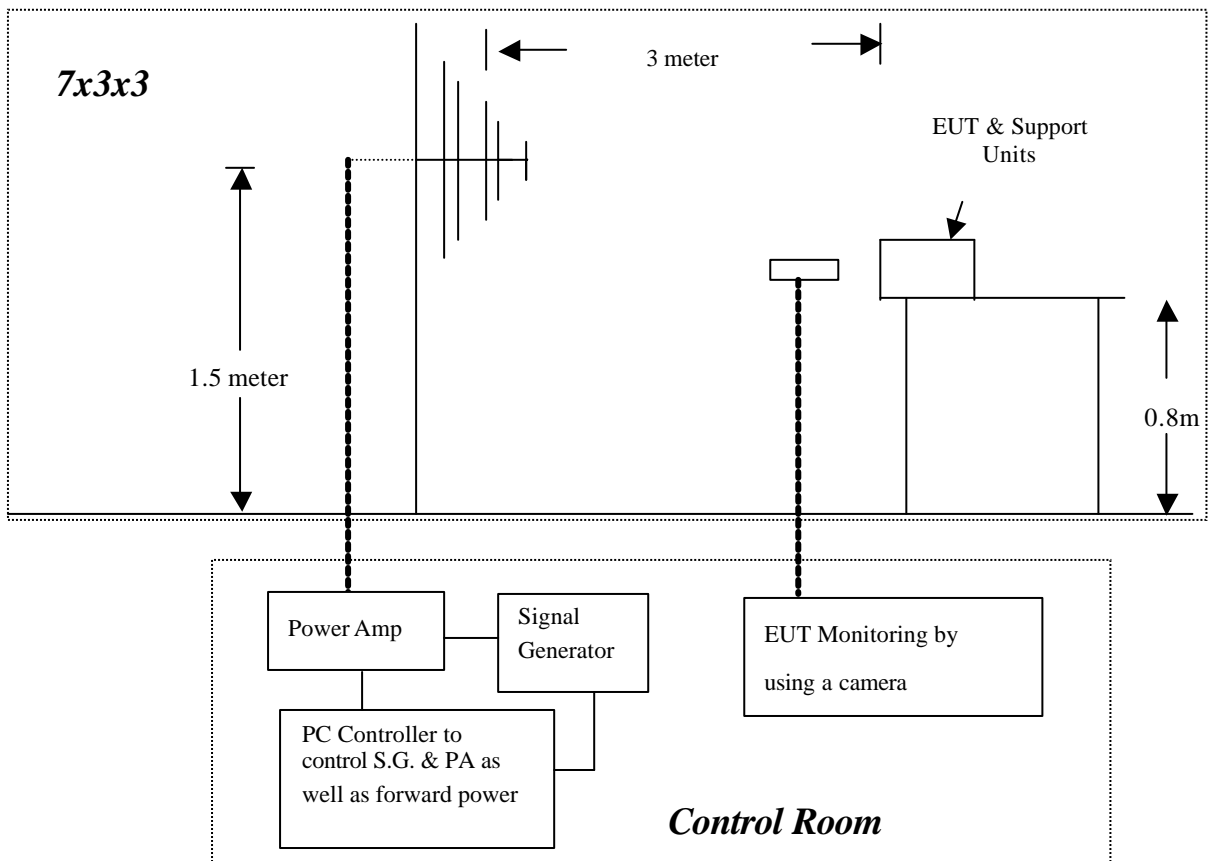



Test Procedure:

Frequency Range 80MHz ~ 2500MHz
Steps : 1 % of fundamental
Dwell Time : 3 sec

| Range (MHz) | Field | Modulation | Polarity | Position | Result (Pass/Fail) |
|-------------|-------|------------|----------|----------|--------------------|
| 80-2500 | 3V/m | Yes | H | 0 | Pass |
| 80-2500 | 3V/m | Yes | V | 0 | Pass |
| 80-2500 | 3V/m | Yes | H | 90 | Pass |
| 80-2500 | 3V/m | Yes | V | 90 | Pass |
| 80-2500 | 3V/m | Yes | H | 180 | Pass |
| 80-2500 | 3V/m | Yes | V | 180 | Pass |
| 80-2500 | 3V/m | Yes | H | 270 | Pass |
| 80-2500 | 3V/m | Yes | V | 270 | Pass |

Observation: No function degraded during the tests.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer' s presets)
- Chang of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.

For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer' s specifications) that does not affect ESSENTIAL PERFORMANCE or



safety.

12 FAST TRANSIENTS/BURST IMMUNITY TEST

Port : AC Power Port and RJ45 Port

Basic Standard : IEC/EN 61000-4-4

Requirements : ± 2 kV for AC Power Port
 ± 0.5 kV for RJ45 Port

Performance Criterion : The Equipment or System shall be able to provide the essential performance and remain safe.


Tested by : BENSON YANG

Temperature : 18°C

Humidity : 53%

Pressure : 1010mbar

Block Diagram of Test Setup:

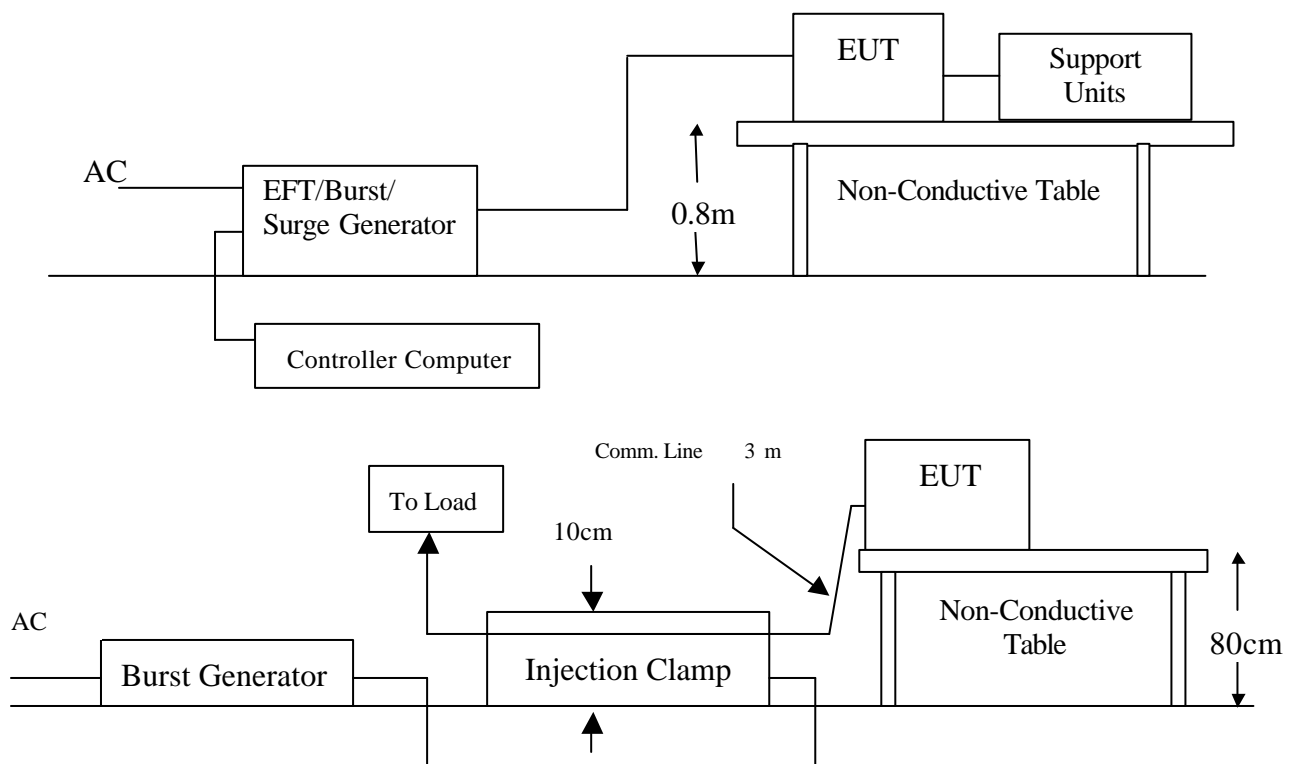



Test Procedure:

Impulse Frequency : 5kHz
Tr/Th : 5/50ns
Burst Duration : 15ms
Burst Period : 300ms

| Inject Line | Voltage kV | Inject Method | Result (Pass/Fail) |
|-------------|------------|---------------|--------------------|
| L | ± 2 | Direct | Pass |
| N | ± 2 | Direct | Pass |
| PE | ± 2 | Direct | Pass |
| L + N | ± 2 | Direct | Pass |
| L + PE | ± 2 | Direct | Pass |
| N + PE | ± 2 | Direct | Pass |
| L + N + PE | ± 2 | Direct | Pass |
| RJ45 | ± 0.5 | Clamp | Pass |

Observation: No function degraded during the tests.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer' s presets)
- Chang of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.


For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer' s specifications) that does not affect ESSENTIAL PERFORMANCE or safety.

13 SURGE IMMUNITY TEST

- Port** : AC Power Port
- Basic Standard** : IEC/EN 61000-4-5
- Requirements** : ± 1 kV(Line to Line) for AC Power Port
 ± 2 kV (Line to Ground) for AC Power Port
- Performance Criteria** : The Equipment or System shall be able to provide the essential performance and remain safe.
- Tested by** : BENSON YANG
- Temperature** : 18°C
- Humidity** : 53%
- Pressure** : 1010mbar

Block Diagram of Test Setup:

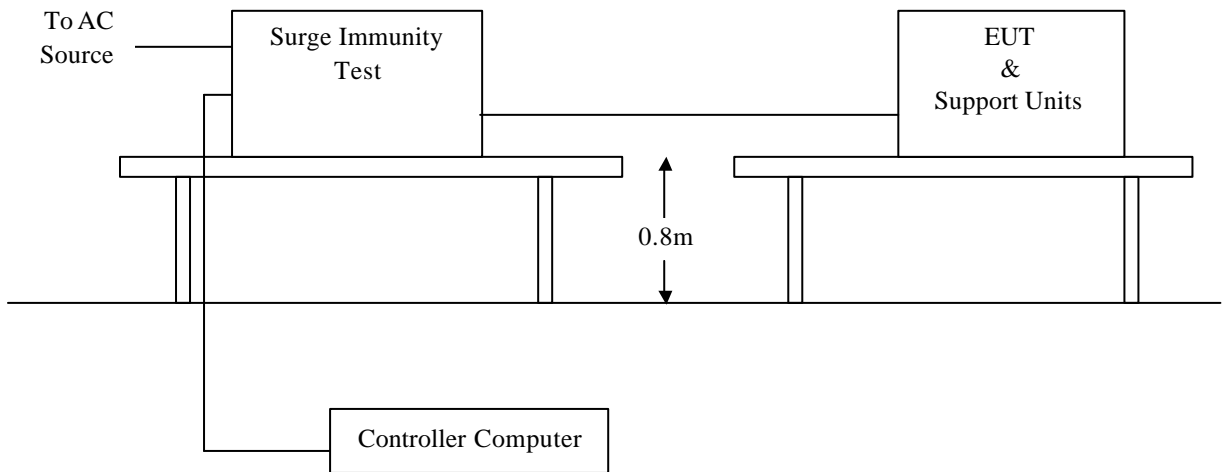



Test Procedure:

Voltage Waveform : 1.2/50 μ s
 Current Waveform : 8/20 μ s
 Polarity : Positive/Negative
 Phase angle : 0°, 90°, 180°, 270°, 359°
 Number of Test : 5

| Coupling Line | Voltage (kV) | Polarity | Coupling Method | Result (Pass/Fail) |
|---------------|--------------|----------|-----------------|--------------------|
| L1-L2 | ±1 | Positive | Capacitive | Pass |
| L1-PE | ±1、 ±2 | Positive | Capacitive | Pass |
| L2-PE | ±1、 ±2 | Positive | Capacitive | Pass |
| L1-L2 | ±1 | Negative | Capacitive | Pass |
| L1-PE | ±1、 ±2 | Negative | Capacitive | Pass |
| L2-PE | ±1、 ±2 | Negative | Capacitive | Pass |

Observation: Where normal functioning of LAN can't be achieved because of the impact of CDN on the EUT, no test be required.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer' s presets)
- Chang of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.


For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer' s specifications) that does not affect ESSENTIAL PERFORMANCE or safety.

14 CONDUCTED DISTURBANCE/INDUCED RADIO-FREQUENCY FIELD IMMUNITY TEST

| | |
|------------------------------|---|
| Port | : AC Power Port and RJ45 Port |
| Basic Standard | : IEC/EN 61000-4-6 |
| Requirements | : 3 V with 80% AM, 1kHz Modulation. |
| Injection Method | : CDN-M3 for AC Power Port CDN-T4 for RJ45 Port |
| Performance Criterion | : The Equipment or System shall be able to provide the essential performance and remain safe. |
| Tested by | : BENSON YANG |
| Temperature | : 18°C |
| Humidity | : 53% |
| Pressure | : 1010mbar |

Block Diagram of Test Setup:

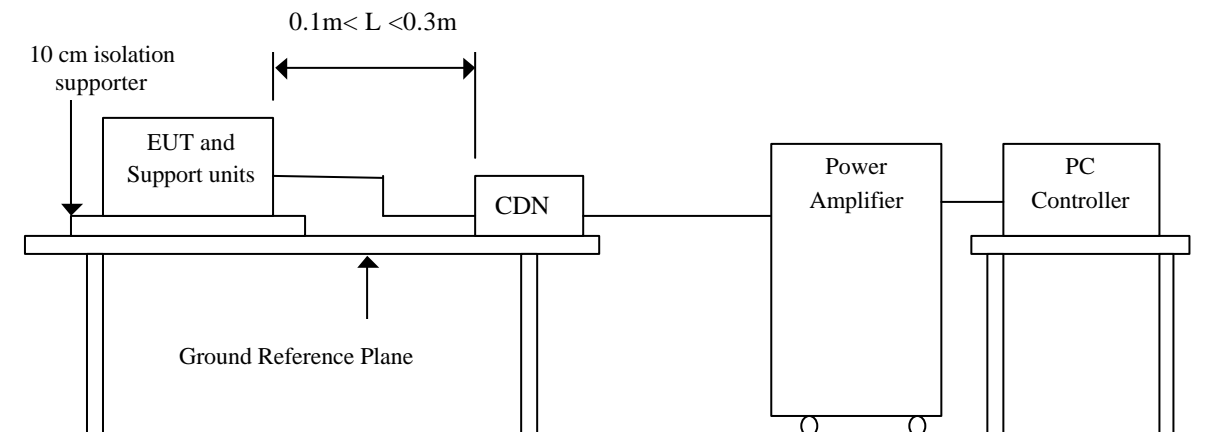



Test Procedure:

Frequency Range : 0.15MHz-80MHz
Frequency Step : 1% of fundamental
Dwell Time : 3 sec

| Range (MHz) | Field | Modulation | Result (Pass/Fail) |
|-------------|-------|------------|--------------------|
| 0.15-80 | 3V | Yes | Pass |

Observation: No function degraded during the tests.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer's presets)
- Change of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.


For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer's specifications) that does not affect ESSENTIAL PERFORMANCE or safety.

15 POWER FREQUENCY MAGNETIC FIELD IMMUNITY TEST

| | |
|------------------------------|---|
| Port | : Enclosure |
| Basic Standard | : IEC/EN 61000-4-8 |
| Requirements | : 3 A/m, 50Hz |
| Performance Criterion | : The Equipment or System shall be able to provide the essential performance and remain safe. |
| Tested by | : BENSON YANG |
| Temperature | : 18°C |
| Humidity | : 53% RH |
| Pressure | : 1010mbar |

Block Diagram of Test Setup:

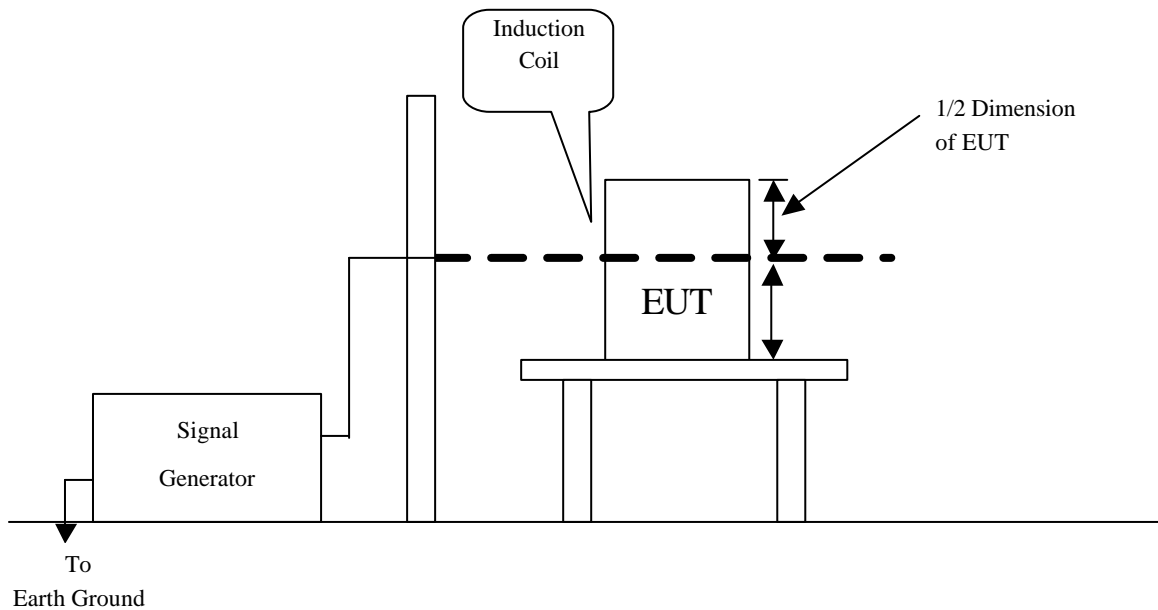



Test Procedure:

Field Strength : 3A/m
Power Freq. : 50Hz, 60Hz
Orientation : X, Y, Z

| Orientation | Field | Result | Remark |
|-------------|------------|--------|--|
| X | 3A/m, 50Hz | Pass | No any function degraded during the tests. |
| Y | 3A/m, 50Hz | Pass | No any function degraded during the tests. |
| Z | 3A/m, 50Hz | Pass | No any function degraded during the tests. |

Observation: No function degraded during the tests.

Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer' s presets)
- Chang of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.

For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer' s specifications) that does not affect ESSENTIAL PERFORMANCE or safety.

16 VOLTAGE DIPS / SHORT INTERRUPTIONS

Port : AC Power Port

Basic Standard : IEC/EN 61000-4-11

Requirement : PHASE ANGLE 0°, 180°

| Voltage Dips | Test Level % U _T | Reduction (%) | Duration (periods) |
|--------------|--------------------------------|------------------|-------------------------|
| | <5 | >95 | 0.5 |
| | 40 | 60 | 5 |
| | 70 | 30 | 25 |

| Voltage Interruptions | Test Level % U _T | Reduction (%) | Duration (second) |
|-----------------------|--------------------------------|------------------|------------------------|
| | <5 | >95 | 5 |

Test Interval : Min. 10 sec.

Performance Criteria : The Equipment or System shall be able to provide the essential performance and remain safe.


Tested by : BENSON YANG

Temperature : 18°C

Humidity : 53%

Pressure : 1010mbar

Block Diagram of Test Setup:

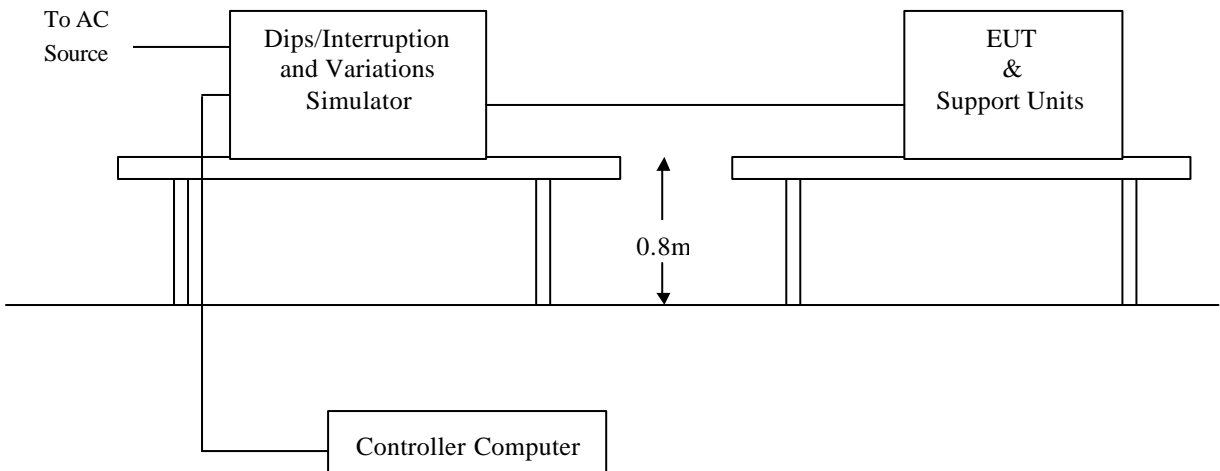



Test Procedure:

The duration with a sequence of three dips/interruptions with interval of 10 s minimums (Between each test event)

Voltage Dips:

| Test Level % U _T | Reduction (%) | Duration (periods) | Observation | Result |
|--------------------------------|------------------|-------------------------|-------------|--------|
| 0 | 100 | 0.5 | Normal | A |
| 40 | 60 | 5 | Normal | A |
| 70 | 30 | 25 | Normal | A |

Voltage Interruptions:

| Test Level % U _T | Reduction (%) | Duration (second) | Observation | Result |
|--------------------------------|------------------|------------------------|---|--------|
| 0 | 100 | 5 | EUT shut down, but EUT can be auto recovered after power turn on. | C |

Note:

1. Normal - No any functions degrade during and after the test.
2. For Voltage Interruption, EQUIPMENT and SYSTEMS are allowed a deviation from the requirements of 36.202.1) at the IMMUNITY TEST LEVEL specified in Table 211, provided the EQUIPMENT or SYSTEM remains safe, experiences no component failures and is restorable to the pre-test state with OPERATOR intervention. Determination of compliance is based upon performance of the EQUIPMENT or SYSTEM during and after application of the test sequence.

Observation: No function degraded during the tests.



Compliance Criteria:

Under the test conditions specified in 36.202, the EQUIPMENT or SYSTEM shall be able to provide the ESSENTIAL PERFORMANCE and remain safe. The following DEGRADATIONS associated with ESSENTIAL PERFORMANCE and safety shall not be allowed:

- Component failures
- Changes in programmable parameters
- Reset to factory defaults (manufacturer' s presets)
- Chang of operating mode
- False alarms
- Cessation or interruption of any intended operation, even if accompanied by an alarm
- Initiation of any unintended operation, including unintended or uncontrolled motion, even if accompanied by an alarm
- Error of a displayed numerical value sufficiently large to affect diagnosis or treatment
- Noise on a waveform in which the noise is indistinguishable from physiologically-produced signals or the noise interferes with interpretation of physiologically-produced signals
- Artefact or distortion in an image in which the artefact is indistinguishable from physiologically-produced signals or the distortion interferes with interpretation of physiologically-produced signals
- Failure of automatic diagnosis or treatment EQUIPMENT and SYSTEMS to diagnose or treat, even if accompanied by an alarm.

For EQUIPMENT and SYSTEMS with multiple FUNCTIONS, the criteria apply to each FUNCTION, parameter and channel.

The EQUIPMENT or SYSTEM may exhibit DEGRADATION of performance (e.g. deviation from manufacturer' s specifications) that does not affect ESSENTIAL PERFORMANCE or safety.

APPENDIX I - PHOTOGRAPHS OF TEST SETUP

LINE CONDUCTED EMISSION TEST (EN 55011)



RADIATED EMISSION TEST (EN 55011)



POWER HARMONIC & VOLTAGE FLUCTUATION / FLICKER TEST



ELECTROSTATIC DISCHARGE TEST



RADIATED ELECTROMAGNETIC FIELD TEST



FAST TRANSIENTS/BURST TEST



FAST TRANSIENTS/BURST TEST (IEC 61000-4-4 FOR I/O)



SURGE IMMUNITY TEST



CONDUCTED DISTURBANCE, INDUCED BY RADIO-FREQUENCY FIELDS TEST



CONDUCTED DISTURBANCE, INDUCED BY RADIO-FREQUENCY FIELDS TEST (IEC 61000-4-6 FOR I/O)



POWER FREQUENCY MAGNETIC FIELD IMMUNITY TEST



VOLTAGE DIPS / INTERRUPTION TEST






APPENDIX II – TEST RESULT OF EN 61000-3-2/-3

Test Result: Pass


Source qualification: Normal

Current & voltage waveforms

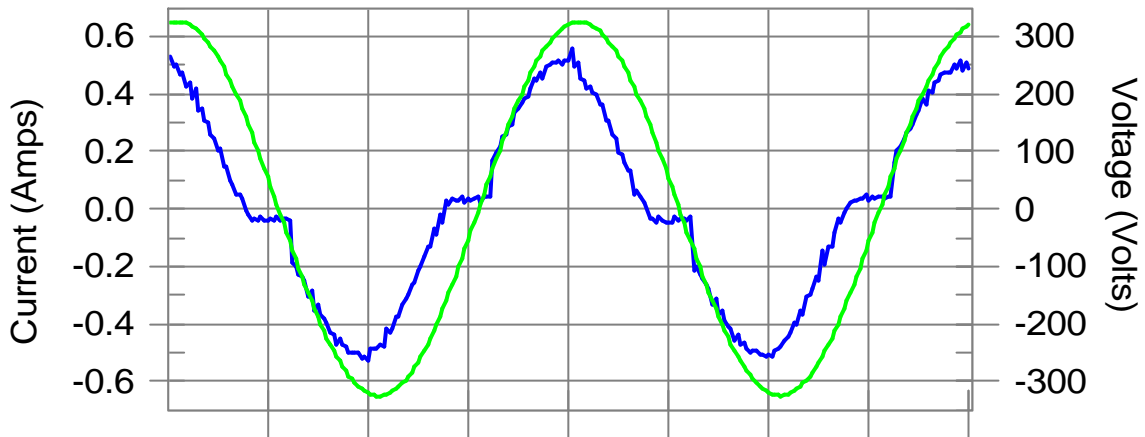

Harmonics and Class D limit line

European Limits

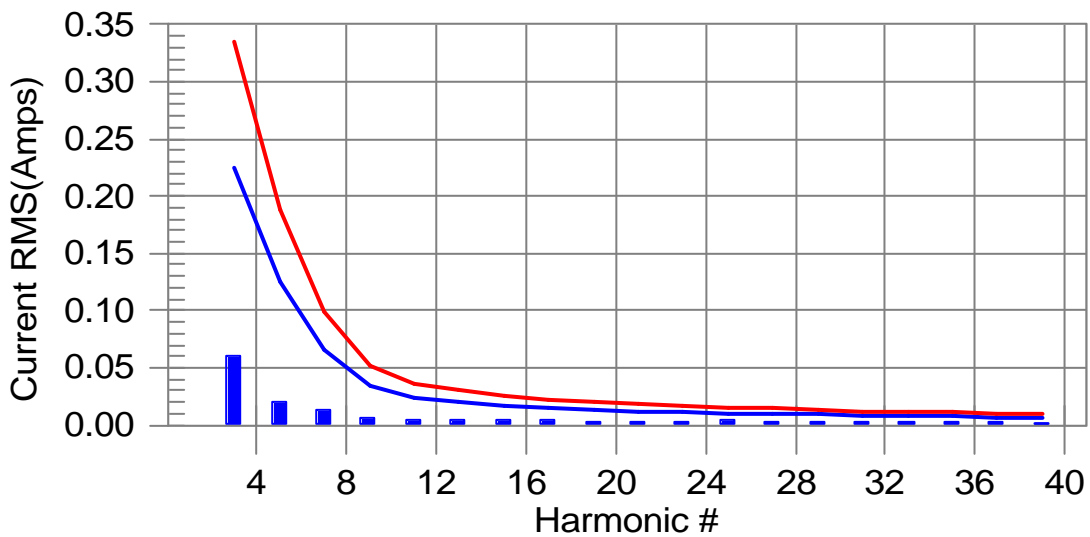

Test result: Pass

Worst harmonic was #25 with 24.61 % of the limit.



Test Result: Pass

Source qualification: Normal

THC(A): 0.066

I THD(pk%): 21.551

POHC(A): N/A

POHC Limit(A): N/A

Highest parameter values during test:

V_RMS (Volts): 230.06

I_Peak (Amps): 0.561

I_RMS (Amps): 0.330

I_Fund (Amps): 0.328

Crest Factor: 1.757

Power (Watts): 72

Power Factor: 0.947

| Harm# | Harms(avg) | 100%Limit | %of Limit | Harms(max) | 150%Limit | %of Limit | Status |
|-------|------------|-----------|-----------|------------|-----------|-----------|--------|
| 2 | 0.000 | | | | | | |
| 3 | 0.059 | 0.225 | 26.3 | 0.060 | 0.334 | 17.90 | Pass |
| 4 | 0.000 | | | | | | |
| 5 | 0.020 | 0.126 | 15.7 | 0.020 | 0.189 | 10.76 | Pass |
| 6 | 0.000 | | | | | | |
| 7 | 0.013 | 0.066 | 19.0 | 0.013 | 0.099 | 13.12 | Pass |
| 8 | 0.000 | | | | | | |
| 9 | 0.006 | 0.034 | 16.4 | 0.006 | 0.051 | 12.70 | Pass |
| 10 | 0.000 | | | | | | |
| 11 | 0.004 | 0.024 | 16.7 | 0.005 | 0.036 | 13.79 | Pass |
| 12 | 0.000 | | | | | | |
| 13 | 0.004 | 0.020 | 17.7 | 0.004 | 0.030 | 13.63 | Pass |
| 14 | 0.000 | | | | | | |
| 15 | 0.004 | 0.017 | 24.5 | 0.005 | 0.026 | 18.02 | Pass |
| 16 | 0.000 | | | | | | |
| 17 | 0.004 | 0.015 | 26.2 | 0.004 | 0.023 | 19.09 | Pass |
| 18 | 0.000 | | | | | | |
| 19 | 0.003 | 0.014 | 23.3 | 0.004 | 0.021 | 17.54 | Pass |
| 20 | 0.000 | | | | | | |
| 21 | 0.002 | 0.012 | 18.5 | 0.003 | 0.019 | 15.45 | Pass |
| 22 | 0.000 | | | | | | |
| 23 | 0.003 | 0.011 | 25.9 | 0.004 | 0.017 | 21.98 | Pass |
| 24 | 0.000 | | | | | | |
| 25 | 0.003 | 0.010 | 30.9 | 0.004 | 0.015 | 24.61 | Pass |
| 26 | 0.000 | | | | | | |
| 27 | 0.003 | 0.010 | 28.4 | 0.003 | 0.015 | 22.51 | Pass |
| 28 | 0.000 | | | | | | |
| 29 | 0.002 | 0.009 | 19.0 | 0.002 | 0.014 | 16.91 | Pass |
| 30 | 0.000 | | | | | | |
| 31 | 0.002 | 0.008 | 27.3 | 0.003 | 0.012 | 20.56 | Pass |
| 32 | 0.000 | | | | | | |
| 33 | 0.002 | 0.008 | 27.1 | 0.002 | 0.012 | 21.17 | Pass |
| 34 | 0.000 | | | | | | |
| 35 | 0.002 | 0.007 | 24.1 | 0.002 | 0.011 | 20.46 | Pass |
| 36 | 0.000 | | | | | | |
| 37 | 0.002 | 0.007 | 25.4 | 0.002 | 0.010 | 19.81 | Pass |
| 38 | 0.000 | | | | | | |
| 39 | 0.002 | 0.007 | 25.3 | 0.002 | 0.010 | 19.53 | Pass |
| 40 | 0.000 | | | | | | |



Test Result: Pass

Source qualification: Normal

Highest parameter values during test:

Voltage (Vrms): 230.06

I_Peak (Amps): 0.561

I_RMS (Amps): 0.330

I_Fund (Amps): 0.328

Crest Factor: 1.757

Power (Watts): 72

Power Factor: 0.947

| Harm# | Harmonics V-rms | Limit V-rms | % of Limit | Status |
|-------|-----------------|-------------|------------|--------|
| 2 | 0.127 | 0.460 | 27.62 | OK |
| 3 | 0.383 | 2.070 | 18.49 | OK |
| 4 | 0.044 | 0.460 | 9.66 | OK |
| 5 | 0.033 | 0.920 | 3.64 | OK |
| 6 | 0.068 | 0.460 | 14.86 | OK |
| 7 | 0.038 | 0.690 | 5.49 | OK |
| 8 | 0.035 | 0.460 | 7.62 | OK |
| 9 | 0.054 | 0.459 | 11.69 | OK |
| 10 | 0.026 | 0.459 | 5.63 | OK |
| 11 | 0.057 | 0.230 | 24.94 | OK |
| 12 | 0.021 | 0.230 | 9.35 | OK |
| 13 | 0.024 | 0.230 | 10.62 | OK |
| 14 | 0.015 | 0.230 | 6.73 | OK |
| 15 | 0.019 | 0.230 | 8.38 | OK |
| 16 | 0.019 | 0.230 | 8.41 | OK |
| 17 | 0.014 | 0.230 | 6.15 | OK |
| 18 | 0.023 | 0.230 | 9.90 | OK |
| 19 | 0.017 | 0.230 | 7.53 | OK |
| 20 | 0.021 | 0.230 | 9.08 | OK |
| 21 | 0.028 | 0.230 | 12.05 | OK |
| 22 | 0.020 | 0.230 | 8.66 | OK |
| 23 | 0.058 | 0.230 | 25.33 | OK |
| 24 | 0.020 | 0.230 | 8.67 | OK |
| 25 | 0.054 | 0.230 | 23.36 | OK |
| 26 | 0.026 | 0.230 | 11.34 | OK |
| 27 | 0.034 | 0.230 | 14.86 | OK |
| 28 | 0.033 | 0.230 | 14.16 | OK |
| 29 | 0.025 | 0.230 | 10.83 | OK |
| 30 | 0.065 | 0.230 | 28.27 | OK |
| 31 | 0.012 | 0.230 | 5.16 | OK |
| 32 | 0.013 | 0.230 | 5.55 | OK |
| 33 | 0.013 | 0.230 | 5.72 | OK |
| 34 | 0.009 | 0.230 | 3.71 | OK |
| 35 | 0.021 | 0.230 | 8.93 | OK |
| 36 | 0.008 | 0.230 | 3.70 | OK |
| 37 | 0.015 | 0.230 | 6.36 | OK |
| 38 | 0.008 | 0.230 | 3.42 | OK |
| 39 | 0.008 | 0.230 | 3.65 | OK |
| 40 | 0.009 | 0.230 | 3.90 | OK |




Test Result: Pass

Status: Test Completed

Pst_i and limit line

European Limits

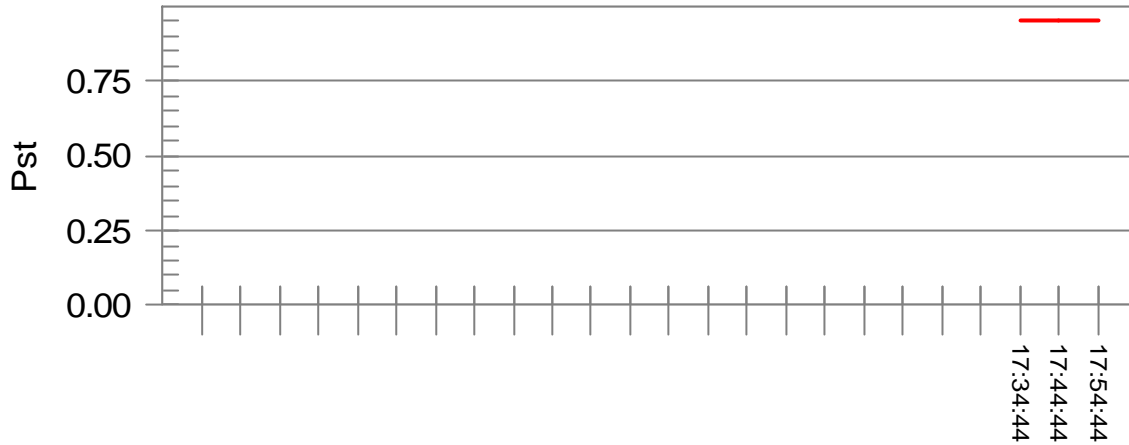

Time is too short for Plt plot

Parameter values recorded during the test:

| | | | | |
|---------------------------------|--------|------------------|-------|------|
| Vrms at the end of test (Volt): | 229.54 | | | |
| Highest dt (%): | 0.00 | Test limit (%): | 3.14 | Pass |
| Time(mS) > dt: | 0.0 | Test limit (mS): | 500.0 | Pass |
| Highest dc (%): | 0.00 | Test limit (%): | 3.14 | Pass |
| Highest dmax (%): | 0.00 | Test limit (%): | 3.80 | Pass |
| Highest Pst (10 min. period): | 0.001 | Test limit: | 0.950 | Pass |
| Highest Plt (2 hr. period): | 0.001 | Test limit: | 0.617 | Pass |