

1. Test item list -----	2
2. Test Configuration -----	3
2. Power On/Off Test -----	4
3. Cold Start and Hot Start Test -----	5
3. Low Temperature Operation Test -----	6
4. High Temp./Humidity Operation Test-----	7
5. Variation Temperature Operation Test -----	8

Test Equipment:

Num	Devices	Model
1.	Programmable Temperature & Humidity Chamber	K.SON. INS. TECH. CORP./THS-D7S-100+1 N2
2.	DC Power Supply	GW Instek PSH-3630
3.	DC Power Supply	Chroma 62012P-600-8

Sample 1 (S/N: 07265848)

Num	Item	Spec
1.	Power Board:	PFM-P13D Rev: A0.2
2.	SubCompact Board:	PFM-550S A1.0-C
	1.CPU	Onboard VIA 533MHz
	2.Memory (Wide Temp.)	Apacer 512MB / ProMOS V54C3256804VDJ71 (PC-133)
	3. CFD	ATP 4GB/ Industrial

Sample 2 (S/N: 07265851)

Num	Item	Spec
1.	Power Board:	PFM-P13D Rev: A0.2
2.	SubCompact Board:	PFM-550S A1.0-C
	1.CPU	Onboard VIA 533MHz
	2.Memory (Wide Temp.)	Apacer 512MB / ProMOS V54C3256804VDJ71 (PC-133)
	3. CFD	ATP 4GB/ Industrial

Sample 3 (S/N: 07265852)

Num	Item	Spec
1.	Power Board:	PFM-P13D Rev: A0.2
2.	SubCompact Board:	PFM-550S A1.0-C
	1.CPU	Onboard VIA 533MHz
	2.Memory (Wide Temp.)	Apacer 512MB / ProMOS V54C3256804VDJ71 (PC-133)
	3. CFD	ATP 4GB/ Industrial

Sample 4 (S/N: 07265853)

Num	Item	Spec
1.	Power Board:	PFM-P13D Rev: A0.2
2.	SubCompact Board:	PFM-550S A1.0-C
	1.CPU	Onboard VIA 533MHz
	2.Memory (Wide Temp.)	Apacer 512MB / ProMOS V54C3256804VDJ71 (PC-133)
	3. CFD	ATP 4GB/ Industrial


Test Date: 06-12~13-2008

Test Site: AAEON QA Internal Lab.

Test Standard: Reference IEC 68-2-1 Testing procedures
Test Ad: Cold Test
Reference IEC 68-2-3 Testing procedures
Test Ca: Damp Heat steady state Test

Test Equipment:
Programmable Temperature & Humidity Chamber
K.SON. INS. TECH. CORP.
Model: THS-D7S-100+1 N2
Date of Calibration: 12/11/06
Serial Number: 3898

- Test Condition:**
1. Test Low Temperature: -40°C
 2. Test High Temp./ Humidity: 85°C / 90%RH
 3. Test Times: 24 hrs
 4. Power On/Off Time: 1min / 3min
 4. Test Software: DOS Mode / Boot Up Record Program ver 1.41
 5. Test Environment Curve:

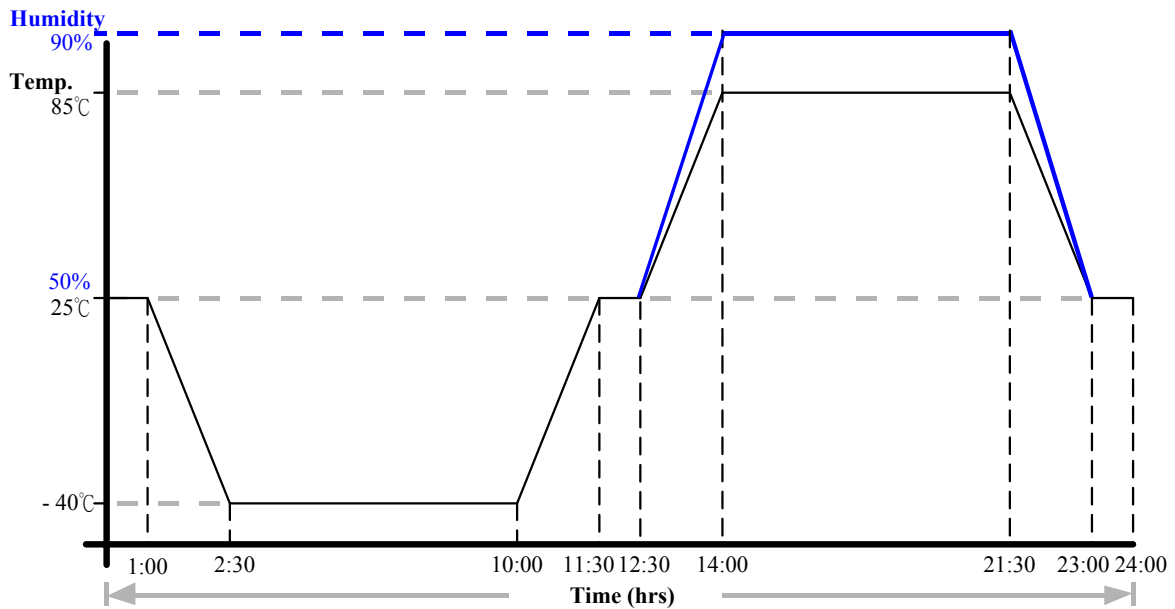

Sample Configuration & Quantity Under Test:
Quantity: 4

Test Result:

No fault was found during the test

Cold start and hot start test


Test Date: 06-9~11-2008

Test Site: AAEON QA Internal Lab.

Test Standard: Reference IEC 68-2-14 Testing procedures
Test N: Change of temperature Test

Test Equipment:
Programmable Temperature & Humidity Chamber
K.SON. INS. TECH. CORP.
Model: THS-D7S-100+1 N2
Date of Calibration: 12/14/06
Serial Number: 3898

Test Condition:

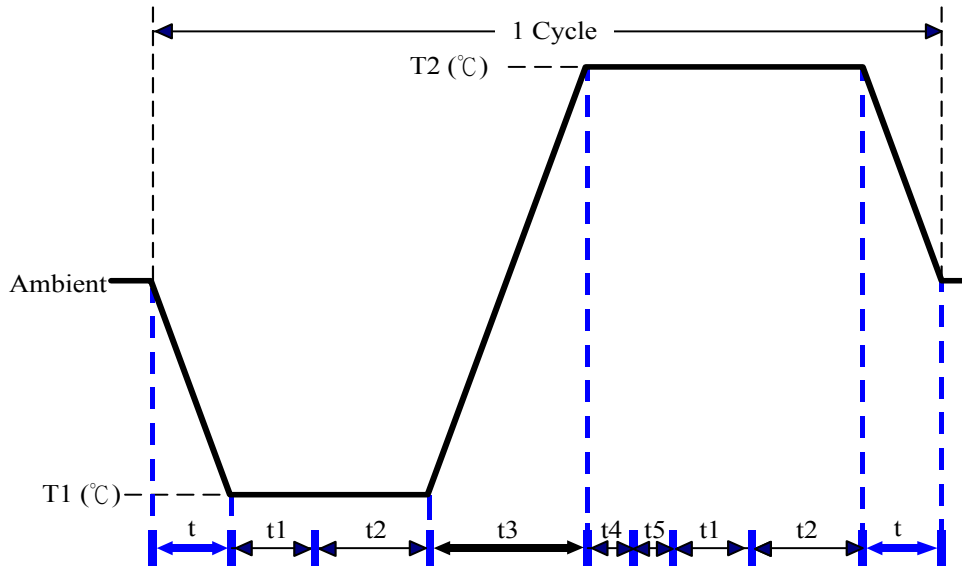

Parameters	Description
T1	-45°C
T2	90°C
t1	1 hrs
t2	2 hrs
t4, t5	30 min
t, t3	2°C/min
n (Cycle)	1

t,t3 = temprature slope
t, t1: Power Off
t2: Power on/off test 10 times (on 2 min / off 5min)
t3,t4: Run PassMark Burn In Test
t5: Win XP Software restart test 2 times
Test Software: Windows XP

Test Result:

No fault was found during the test

Test Date: 06-5~6-2008

Test Site: AAEON QA Internal Lab.


Test Standard: Reference IEC 68-2-1 Testing procedures
Test Ad: Cold Test

Test Equipment:

Programmable Temperature & Humidity Chamber
K.SON. INS. TECH. CORP.
Model: THS-D7S-100+1 N2
Date of Calibration: 12/11/06
Serial Number: 3898

Test Condition:

1. Test Temperature: -40°C, -45°C
2. Test Times: -40°C/24Hrs; -45°C/4Hrs
3. Test Software: Windows XP
4. Test Environment Curve:

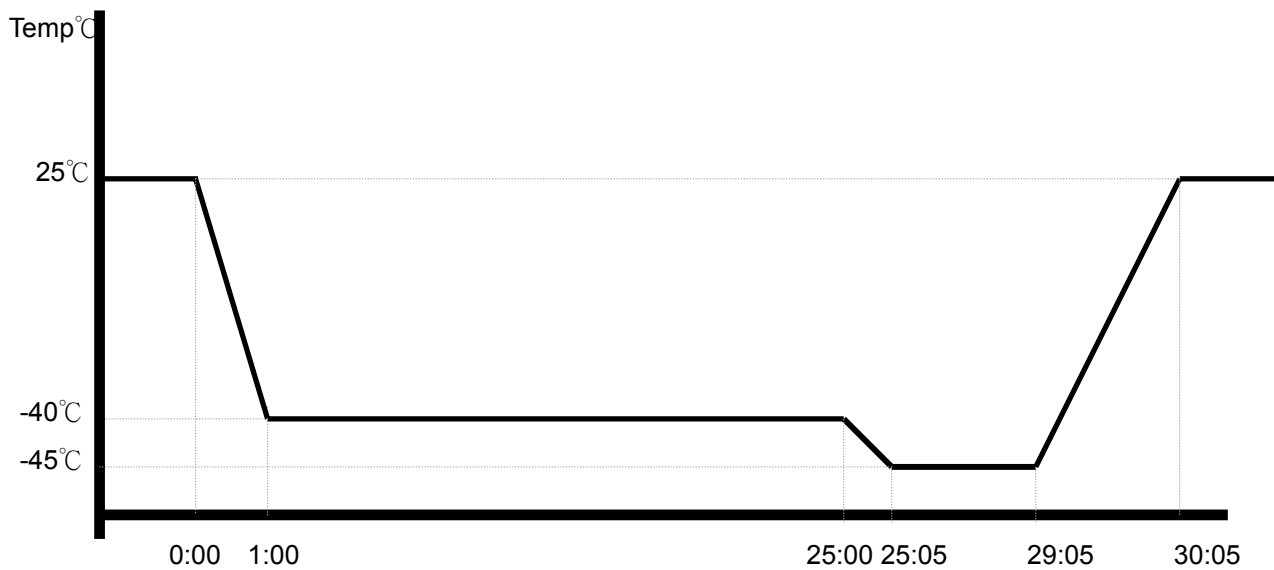

Sample Configuration & Quantity Under Test:

Quantity: 4

Test Result:

No fault was found during the test


Test Date: 06-3~4-2008

Test Site: AAEON QA Internal Lab.

Test Standard: Reference IEC 68-2-3 Testing procedures
Test Ca: Damp Heat steady state Test

Test Equipment:
Programmable Temperature & Humidity Chamber
K.SON. INS. TECH. CORP.
Model: THS-D7S-100+1 N2
Date of Calibration: 12/11/06
Serial Number: 3898

- Test Condition:**
1. Test Temperature: 85°C, 90°C
 2. Test Humidity: 90%RH
 3. Test Times: 85°C/24Hrs; 90°C/4Hrs
 4. Test Software: Windows XP
 5. Test Environment Curve:

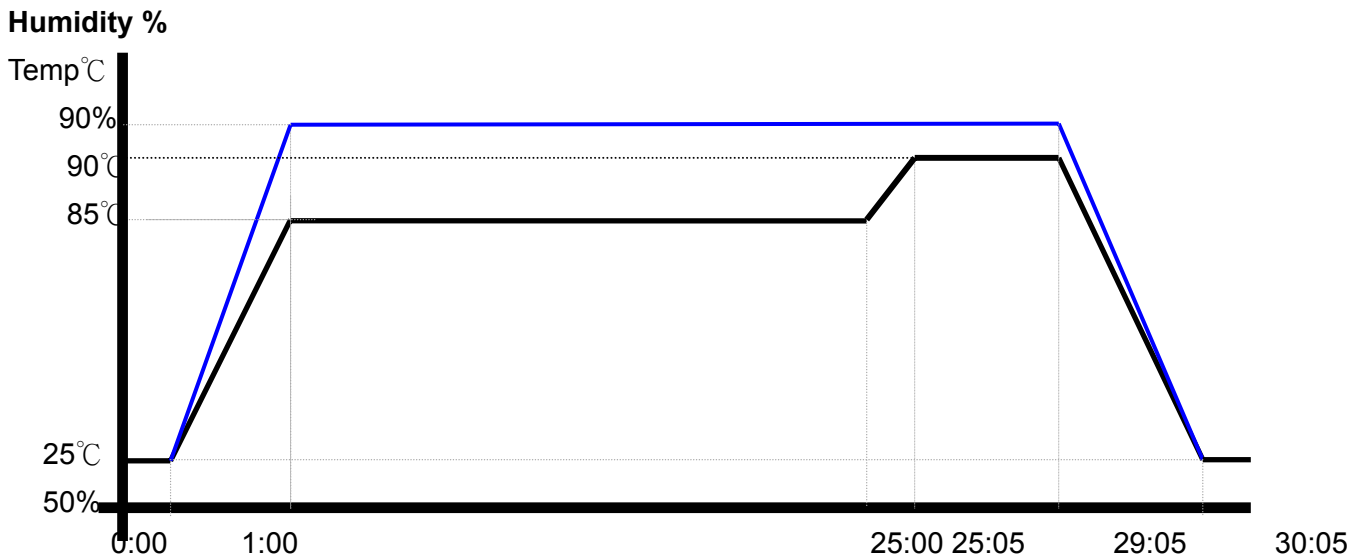

Sample Configuration & Quantity Under Test:

Quantity: 4

Test Result:

No fault was found during the test


Test Date: 06-16~19-2008

Test Site: AAEON QA Internal Lab.

Test Standard: Reference IEC 68-2-14 Testing procedures
Test N: Change of temperature Test

Test Equipment:
Programmable Temperature & Humidity Chamber
K.SON. INS. TECH. CORP.
Model: THS-D7S-100+1 N2
Date of Calibration: 12/11/06
Serial Number: 3898

Test Condition:

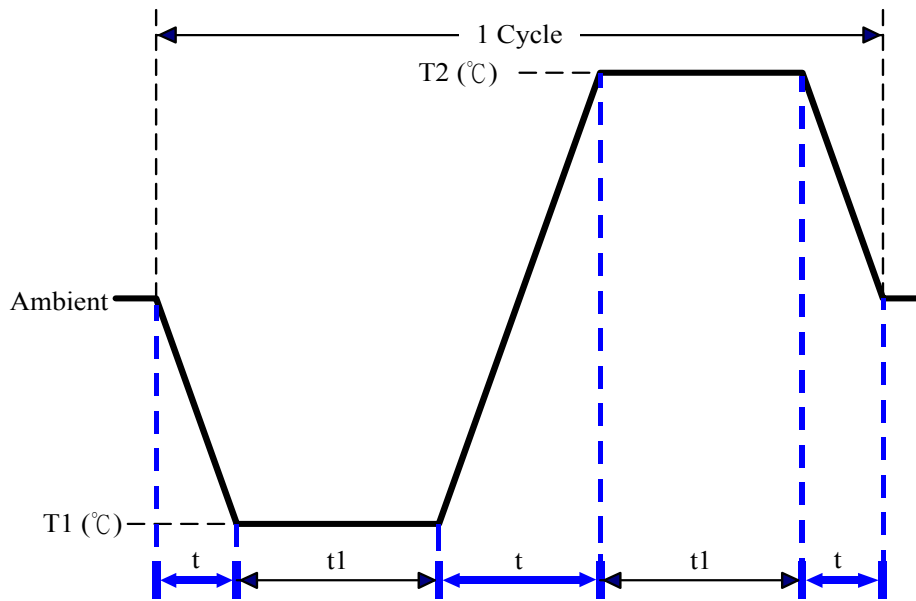

Parameters	Description
T1	-40°C
T2	85°C
t1	3 hrs
t	15°C / min
n (Cycle)	10

t = temprature slope
t1 = means one full cycle test
Test Software: Windows XP

Sample Configuration & Quantity Under Test:
Quantity: 4

Test Result:
No fault was found during the test