


1. Test item list -----	2
2. Random Vibration Operation Test -----	3

Test Configuration:

Num	Item	Spec
1.	Low Noise Medical Station:	Onyx-215
	1.LCD	LCD.15".CPT.CLAA150XP03.Ver1.0-040206.4LAMP
	2.Power Adapter	EDAC EA1050A-120
	3. Inverter	INVERTER Cable.6P 2.00mm.5P 2.00mm.30cm
	4. A/D Board	BT-R08LDNQ REV:05
	5. USB Transfer Board	T040 REV:A02
	6. USB Board	1907YC0301 REV:A1.0
	7. CD-ROM Transfer Board	1907T04101 REV:A0.2
	8. Smart card Board	MR0103
	9. Card Reader Board	GS-2004-CR18801 V1.1
	10. CD-ROM	TEAC DW-224E
2.	Test System	Onyx-153D (PCM-8200 Rev: A1.0 / 512MB / BIOS:1.0)

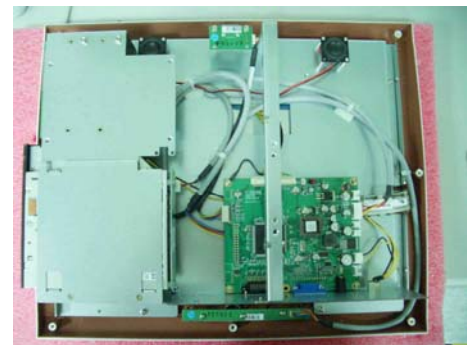

Test Date: 02-21-2006

Test Product: Onyx-215

Test Site: AAEON QA Internal Lab.

Performed By: Rex Chang


Test Standard: Reference IEC68-2-64 Testing procedures
Test Fh: Vibration boardband random test

Test Equipment:

Vibration Simulator System
KING DESIGN Co. LTD.
Model: KD 9363-EM-600F2K-40N20
Serial Number: UU110099090
Date of Calibration: 10/20/2005

Test Condition:

1. Operation
2. Test Acceleration: 1.5 G Random
3. Test Frequency: 5-500Hz
4. Test Axis: X, Y, Z axes
5. Test Time: 60min each axis
6. Test Software: Windows XP / Run one Microsoft media player simultaneously.
7. Test Vibration Curve:

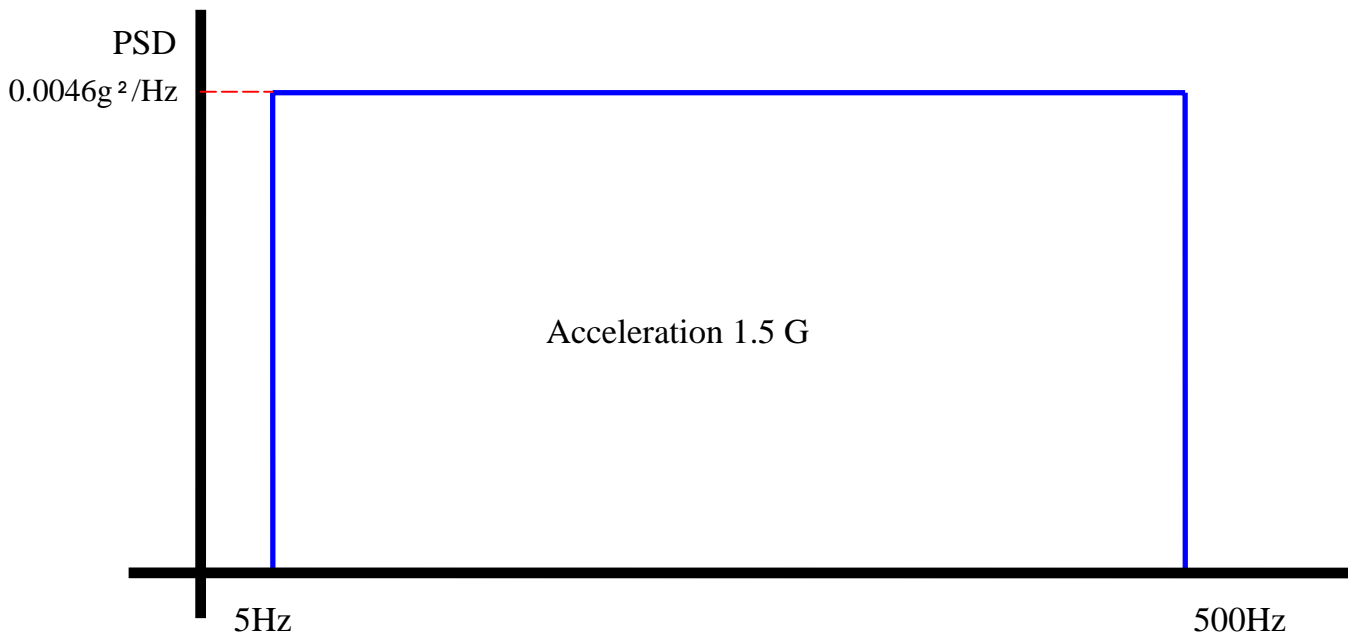

Test Result:

The system structure doesn't deformation; Function is passed during system test.