



Industrial Computing Platform Partner

Onyx-219

Vibration Test Report

Report NO: 06P030019

Issued by: Rex Chang / 10/24/2006
Engineer

Reviewed by: Wenyuan Yang / 10/24/2006
Manager

1. <i>Test item list</i> -----	2
2. <i>Random Vibration Operation Test</i> -----	3

Test Configuration:

Num	Item	Spec
1.	Low Noise Medical Station:	Onyx-219
	1.LCD	TFT LCD.19". AU M190EN04 V7
	2.Power Adapter	SINPRO MPU50-105
	3. Inverter	INVERTER HWA YOUN QF132V1.16 (4LAMPS).
	4. A/D Board	BT-R08LDNQ REV:05
	5. USB Transfer Board	T040 REV: A1.1
	6. USB Board	1907YC0301 REV: A1.0
	7. CD-ROM Transfer Board	1907T04102 REV: A1.0
	8. Smart card Board	MR0103
	9. Card Reader Board	GS-2004-CR18801 V1.1
	10. CD-ROM	TEAC DV-28SL
2.	Test System	AEC-6900 / 256MB(PC133) / BIOS:1.0)

Test Date: 10-23~24-2006

Test Product: Onyx-219

Test Site: AAEON QA Internal Lab.

Performed By: Rex Chang


Test Standard: Reference IEC68-2-64 Testing procedures
Test Fh: Vibration boardband random test

Test Equipment:

Vibration Simulator System
KING DESIGN Co. LTD.
Model: KD 9363-EM-600F2K-40N20
Serial Number: UU110099090
Date of Calibration: 10/17/2006

Test Condition:

1. Operation
2. Test Acceleration: 1.5 G Random
3. Test Frequency: 5-500Hz
4. Test Axis: X, Y, Z axes
5. Test Time: 60min each axis
6. Test Software: Windows XP / Run one Microsoft media player simultaneously.
7. Test Vibration Curve:

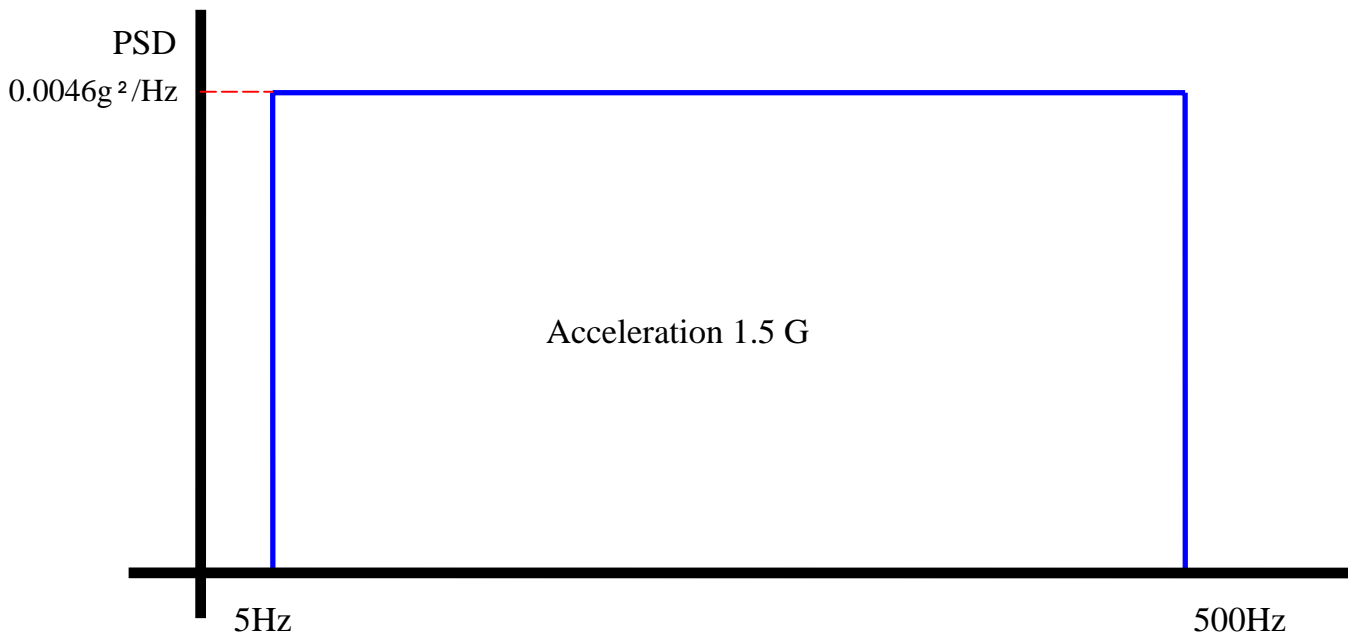

Test Result:

No problem was found during random vibration operation test.